

SU7000 FE-SEM User Manual(Eng.)

울산과학기술원 연구지원본부 기기분석실 UNIST Central Research Facilities UNIST Materials Characterization Lab

#### **CONTACT**

**Ulsan National Institute of Science and Technology** 

Address 50 UNIST-gil, Ulju-gun, Ulsan, 44919, Korea Tel. +82 52 217 0114 Web. www.unist.ac.kr

**UCRF** 

Bldg.102 209

**Tel.** +82 52 217 4028

Web. http://ucrf.unist.ac.kr



## Index

2. UCRF SEM feature	1.	Lab safety	03
1) What to prepare for SEM imaging	2.	UCRF SEM feature	04
<ol> <li>Specimen preparation</li></ol>	3.	SEM operation	05
<ul> <li>3) Starting instrument</li></ul>		1) What to prepare for SEM imaging	05
<ul> <li>4) Coating</li></ul>	ı	2) Specimen preparation	06
<ul> <li>5) Specimen preparation</li></ul>	ı	3) Starting instrument	07
<ul><li>6) Size &amp; height of stub</li></ul>	•	4) Coating	08
7) Loading the holder	ı	5) Specimen preparation	09
8) Setting the storage location	(	6) Size & height of stub	10
9) Acceleration voltage & Probe current		7) Loading the holder	11
	•	8) Setting the storage location	13
10) Beam on		9) Acceleration voltage & Probe current	14
		10) Beam on	15
11) Finding the specimen		11) Finding the specimen	16

12) Focus	18
13) Stigmator	19
14) Working distance	20
15) Beam alignment	21
16) Saving the image	24
17) Finish	26
18) Retrieving the holder	28
19) Transfer SEM data	29
20) Daily check list in lab	30
21) If you encounter a problem while using SEM	31
4. EDS operation	34
5. Access permission application	47
6. Self-user penalty	58

#### Lab Safety

#### Compliance with lab safety rules

If you do not follow the lab safety rules, access and use of the lab will be restricted, so we ask for your cooperation.







No Food or Drink

**Wear Protective Clothes** 


**Wear Foot Protection No Open-Toe Shoes** 

If you didn't bring your lab coat, please wear a shared lab coat entrance side of the room 101-2 on the first basement floor of 102 building.

Make sure to wear a lab coat and enter the lab of UCRF.

Make sure to keep the lab clothes you wore in their original place.

## Lab emergency evacuation

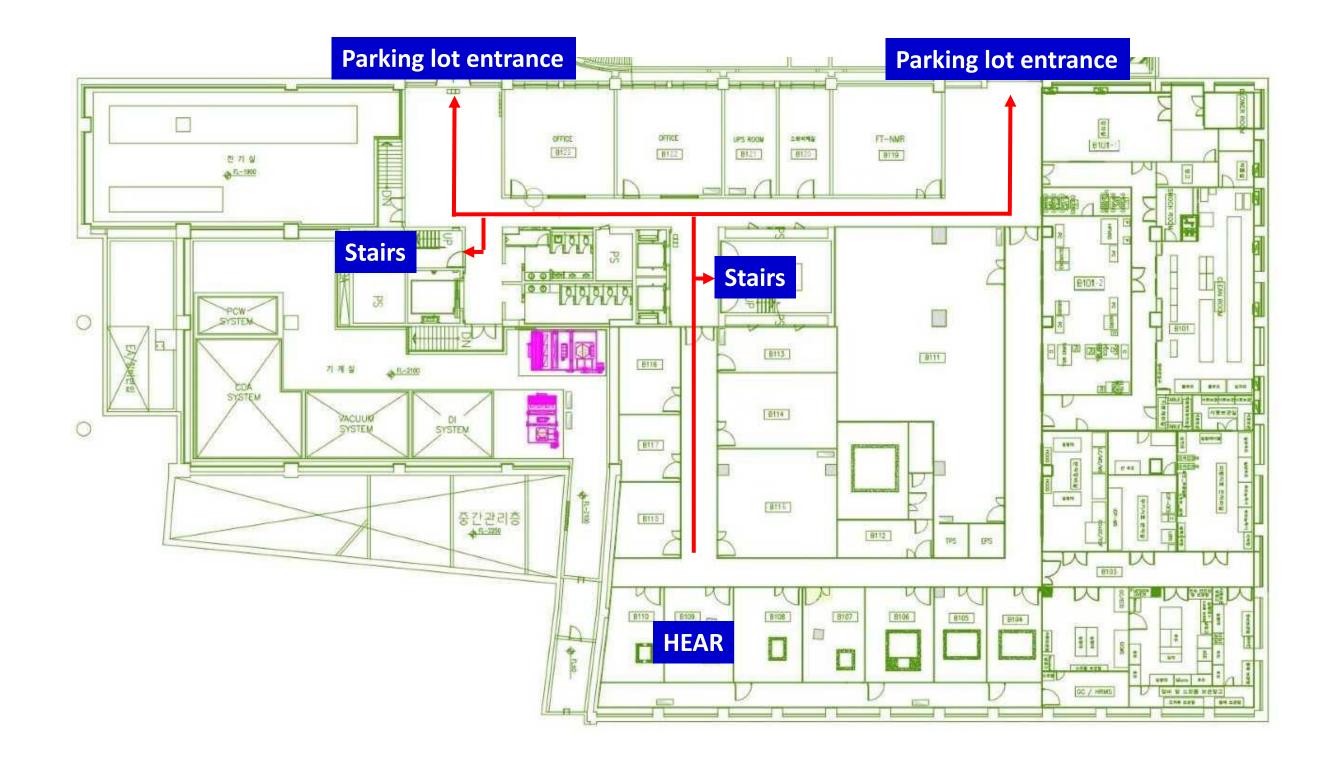



## **UCRF SEM Feature**

	High resolution imaging	EDS analysis	Specimen damage & charge-up	BSE detector	E-SEM	Reservation status	Introduction year	Fee(100%)
Verios FE-SEM			Slight	0	X	Not busy	2024	Undecided
SU8220 cold FE-SEM		0	Slight	X	X	Busy	2013	40,710won /30min
SU7000 FE-SEM	0	0	Serious	X	X	Busy	2021	40,710won /30min
Cold FE-SEM	0	0	Slight	X	X	Not busy	2011	31,320won /30min
Quanta200 FE-SEM	X		Slight	0	0	Not busy	2009	26,100won /30min



#### What to prepare for SEM imaging

- 1. Fully dried samples
- 2. A stub suitable for the equipment and measurement purpose

Туре	Α	В	С	D	
Equipment	SU7000	old FE-SEM FE-SEM E-SEM	Nano FE-SEM Quanta FE-SEM		
Usage	General	Cross section	General	Cross section	
Picture (Front)					
Picture (Back)					

- If you need a special stub other than the stub beside, please discuss with the SEM manager and UDMC.


SEM stub Production


- UDMC Cha Jae-hoon

3. Conductive double-sided carbon tape for SEM



#### **Specimen Preparation**

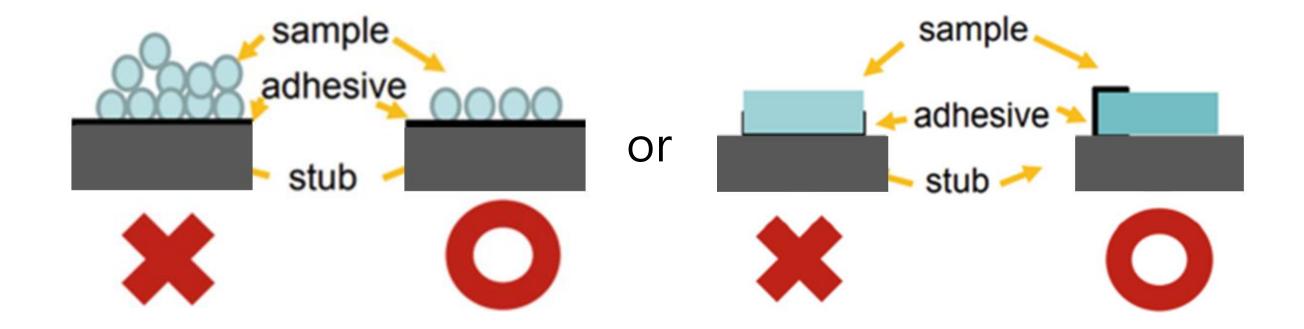


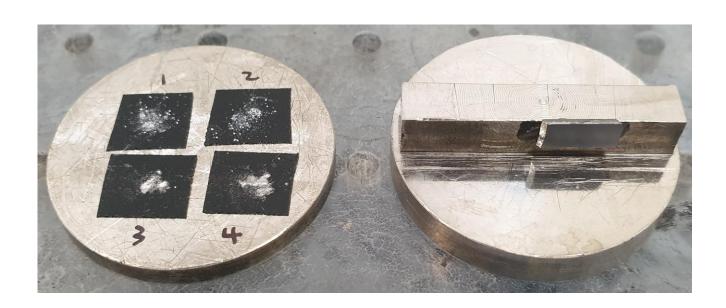

- Sample preparation should be performed by individual laboratories. ★
- 2. Wear appropriate safety gear.(goggles, gloves, etc.)★
- 3. Prepare completely dried specimens.
- 4. Clean the stub with ethanol, etc.
- 5. Attach conductive double-sided tape to the stub and fix a very small amount of specimen to the tape.(For powder samples, be sure to use carbon tape)★
- 6. Blow to remove dust from the specimen. \*
- 7. Coat it if necessary.



#### **Starting Instrument**

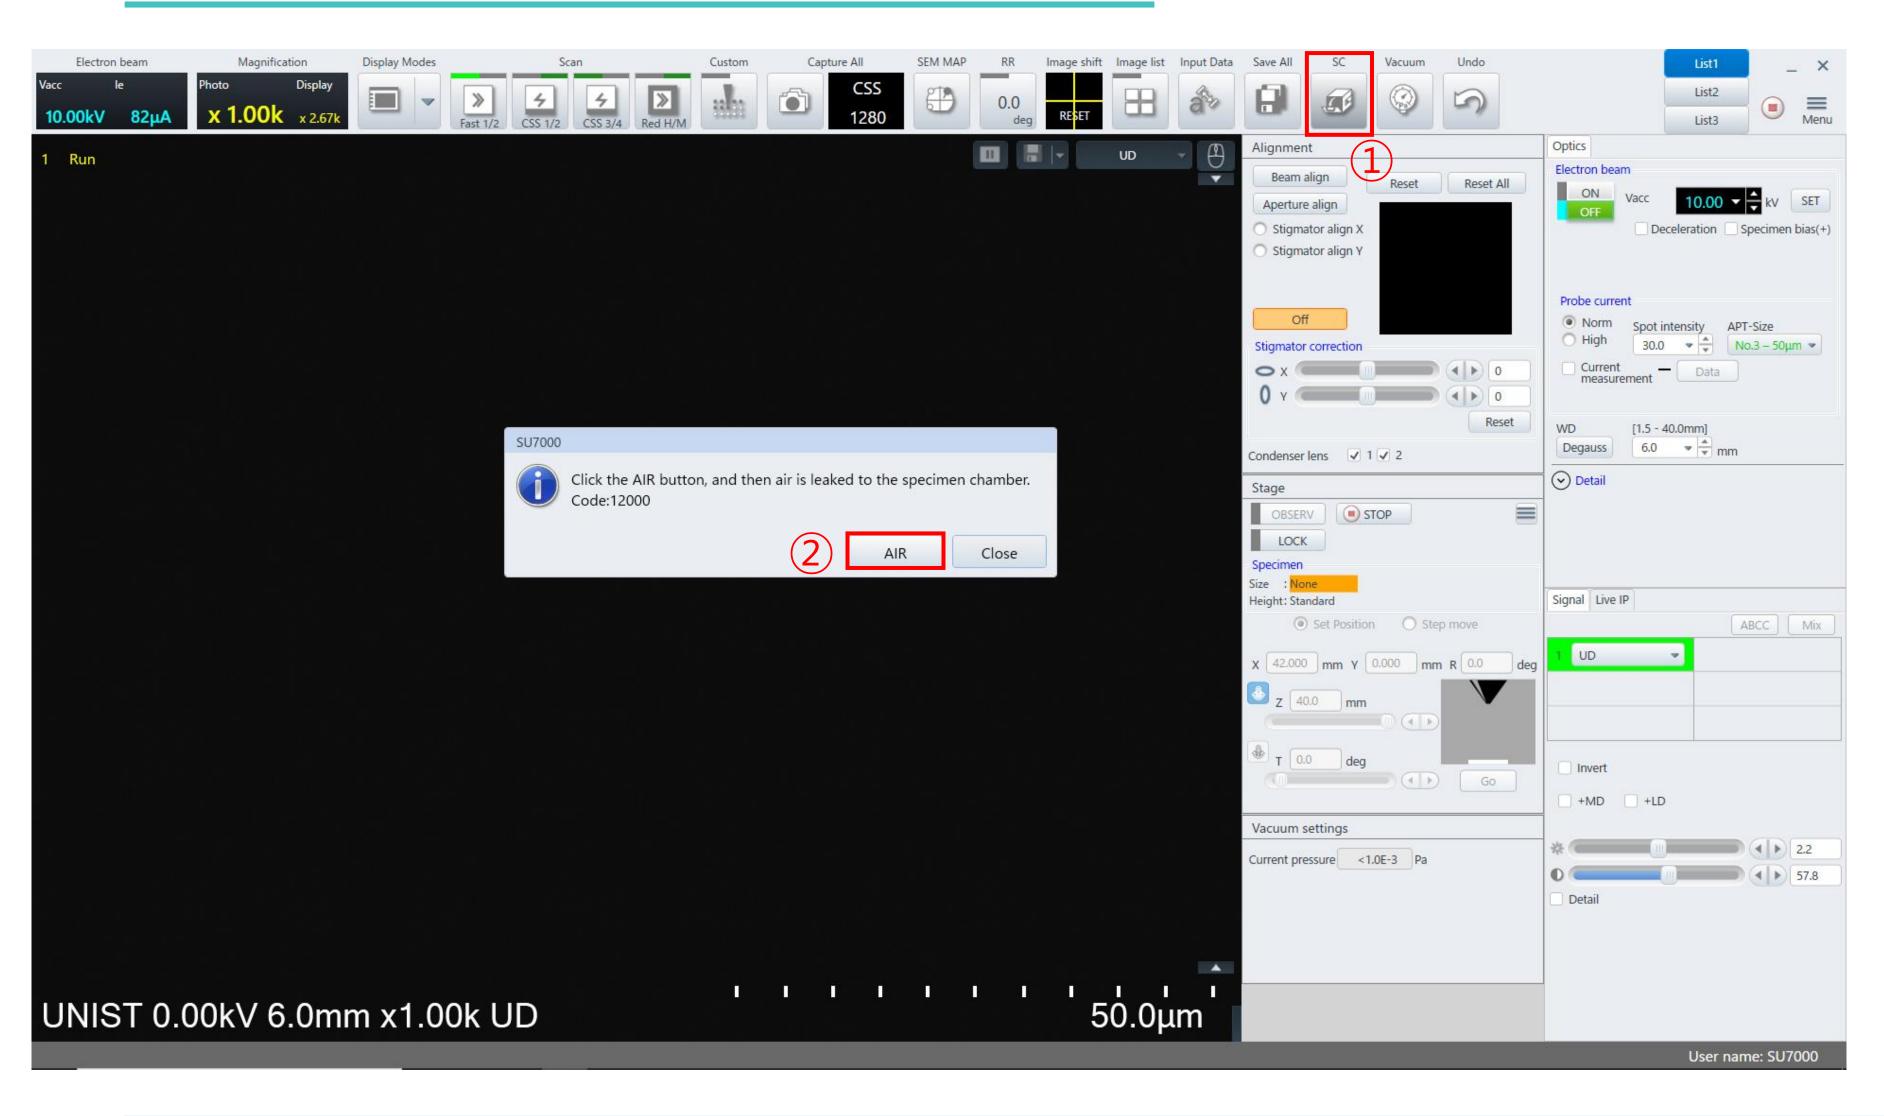


- Double-click the [SU7000] icon.
- 2. Enter your lab ID and PW.
- 3. Click [START] [OK] -[SC] [AIR].
- 4. Prepare the psalm until the buzzer sounds.
- 5. Coating is performed if necessary.



## Coating

#### Hitachi Sputter

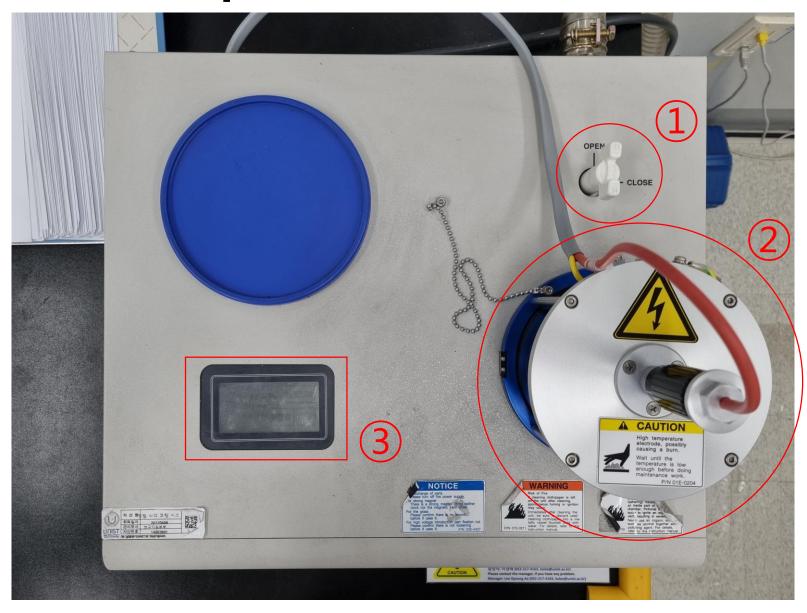

Coating rate

- Pt target: 15 nm/min

<Condition>

- Sputter current: 40mA

- Distance between target and sample: 20 mm


- 1. Reserve and use the equipment.(Zero tolerance)
- 2. Turn the valve open.
- Open the column part and place the specimen in the center.
- 3. Make sure the specimen touches the Pt source.
- 4. Press the touchscreen to view the coating parameters.
- 5. If you want to change a parameter, press [Change].
- 6. Tap each parameter and enter the desired value.
- 7. Press [Enter] [Back] [Start].
- 8. When Processing finished appears on the screen, open the column and remove the specimen.
- Press [Restart], then press [Stop] after 20 seconds.
- 10. Turn the valve to [CLOSE].




#### **Specimen Preparation**






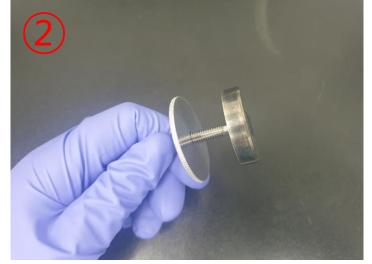



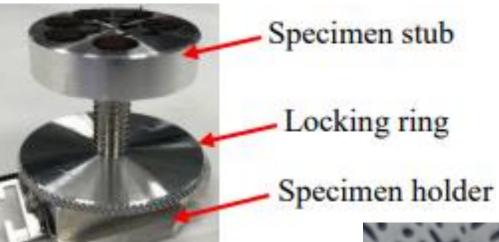




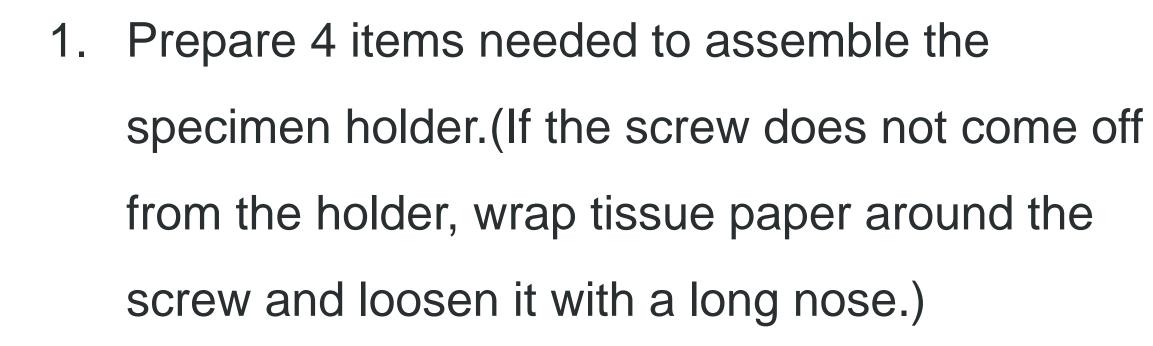


- 2. Assemble the holder in the order shown in the photo below.
- 3. Check if the top and bottom direction of the specimen holder is correct.
- Check if the screw protrudes from the bottom.
- 5. Adjust the specimen height so that the highest part of the specimen touches the height checker.



#### Size & Height of Stub

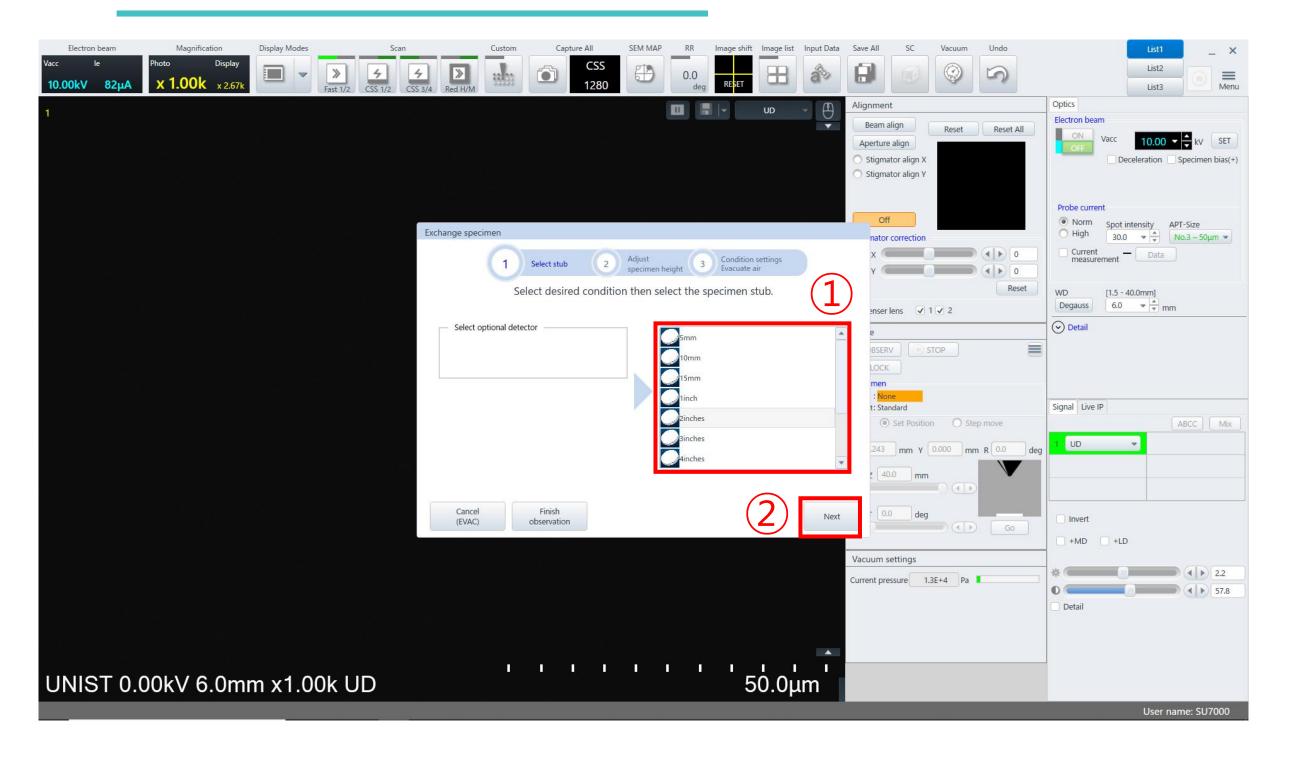


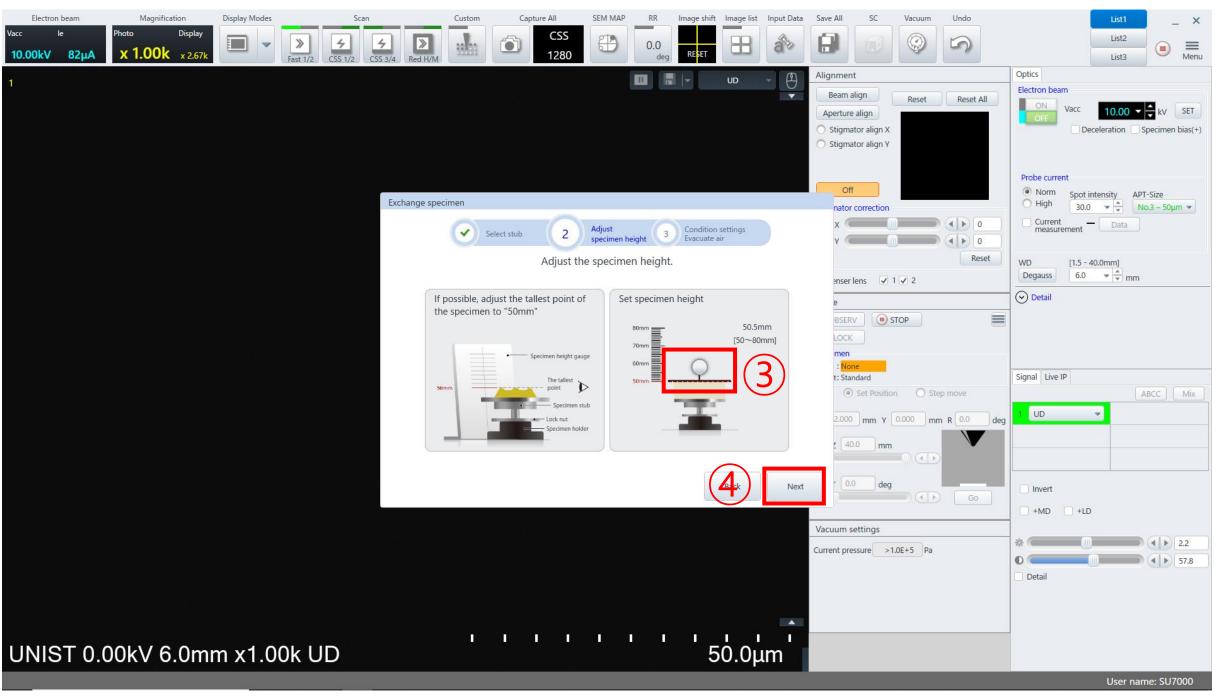

- 1. Select the diameter of the stub one size larger.★
- 2. Click [Next].
- 3. Drag the white circle to 50mm.★
- 4. Click[Next].




#### Loading the Holder

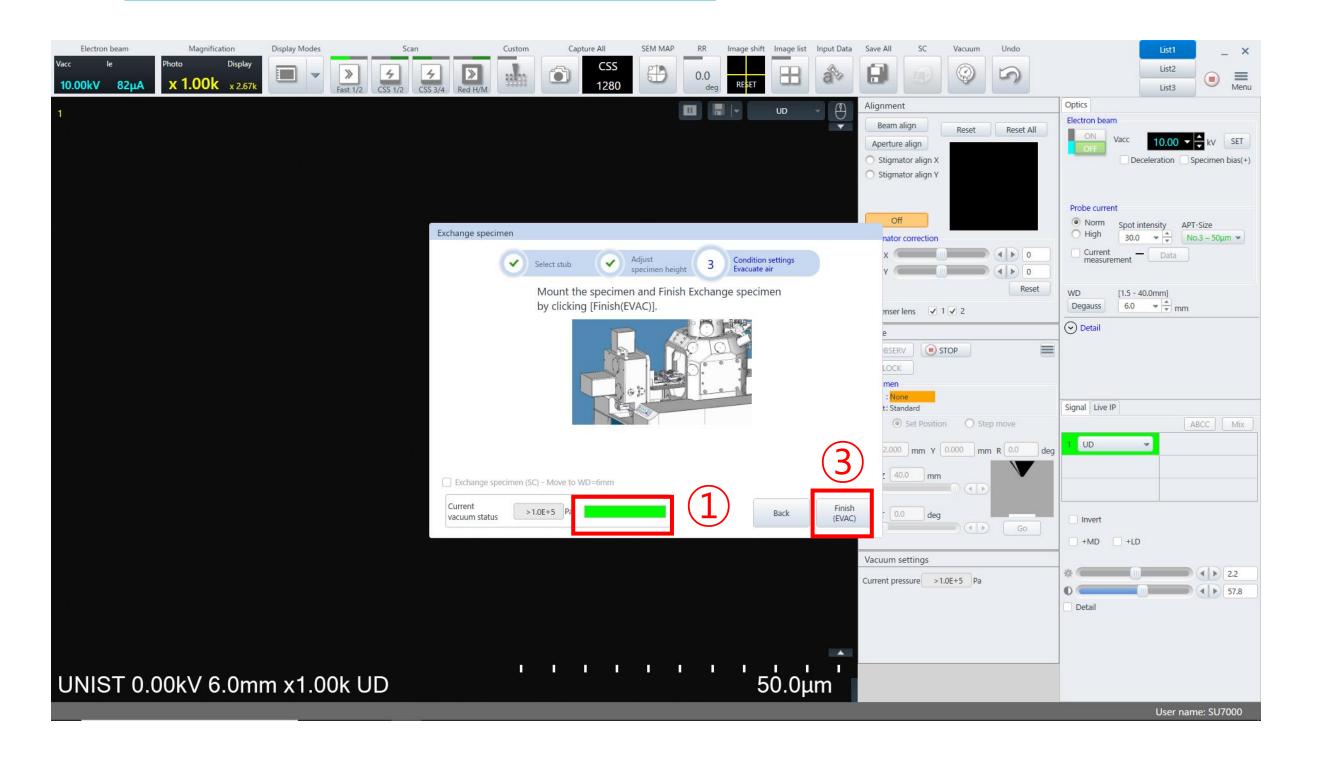




- 1. Wait until the bar in Current vacuum status turns completely green.★
- 2. Open the chamber by pulling the handle.
- 3. Attach the holder to the equipment and close the chamber door.
- 4. While gently pressing the chamber door, click [Finish (EVAC)].


#### **Loading the Holder**

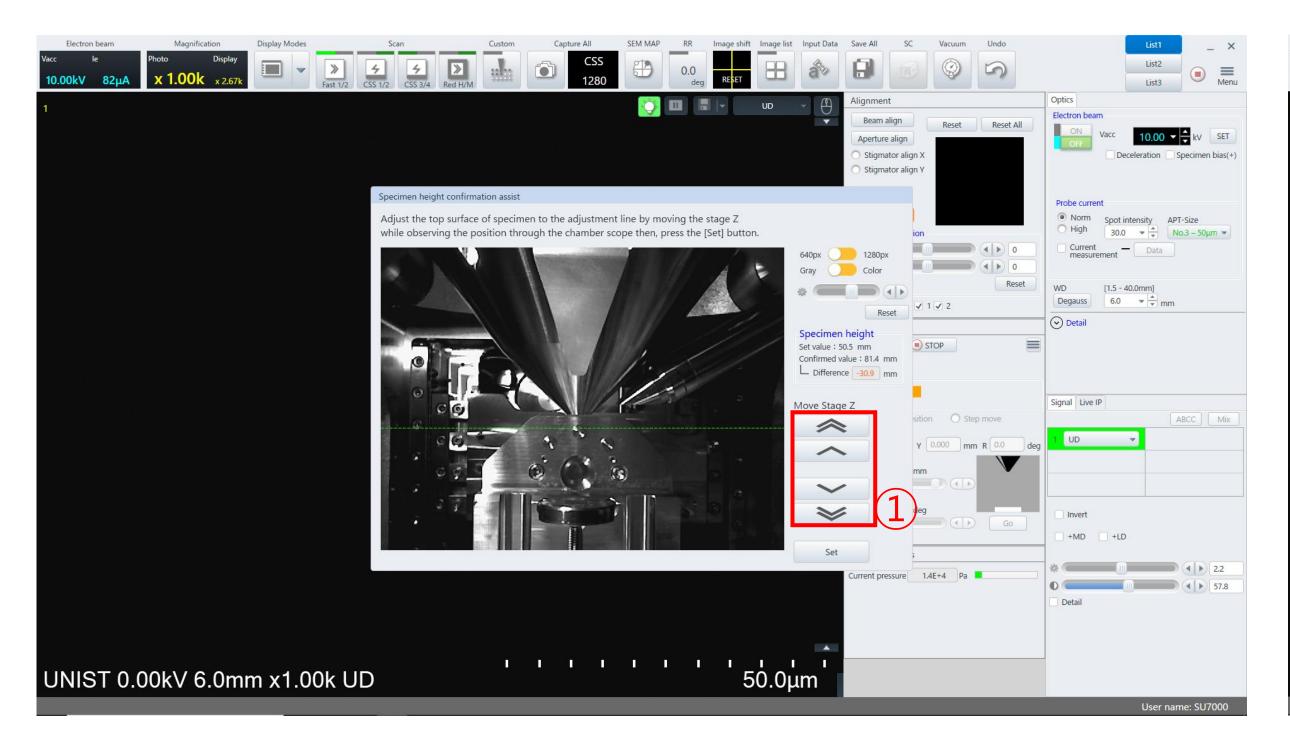


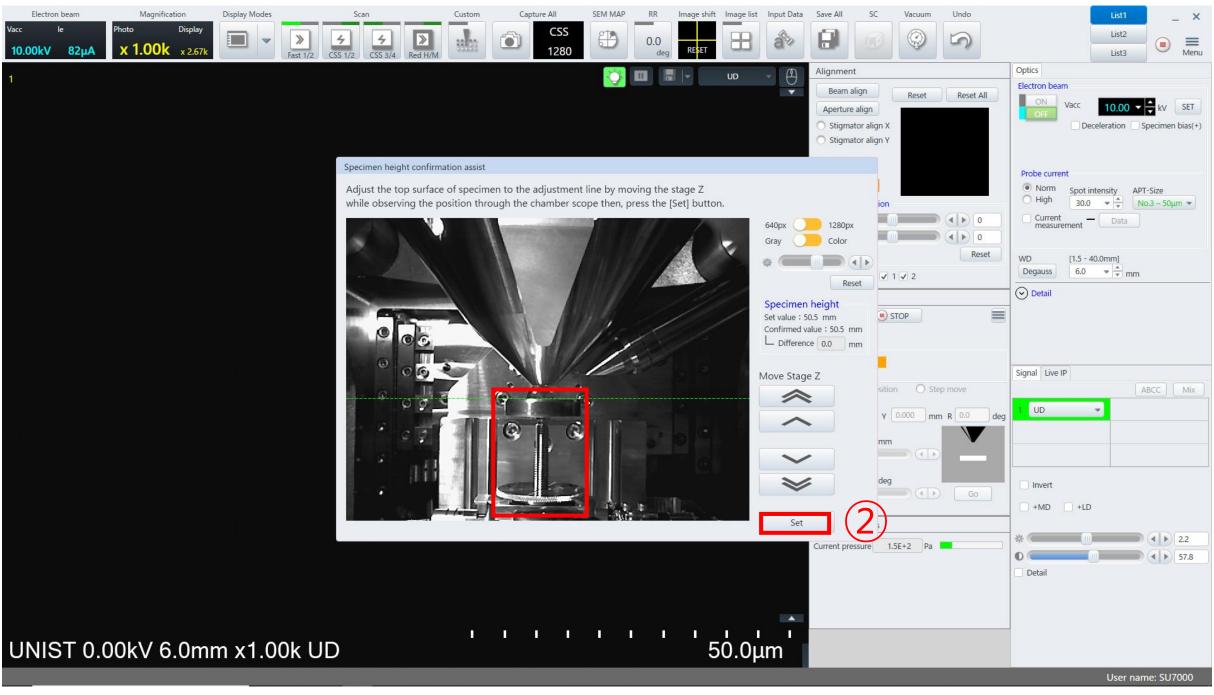

- 1. Keep pressing the arrow so that the highest part of the specimen is on the green line.
- 2. Click [Set].


#### **Setting the Data Storage Location**

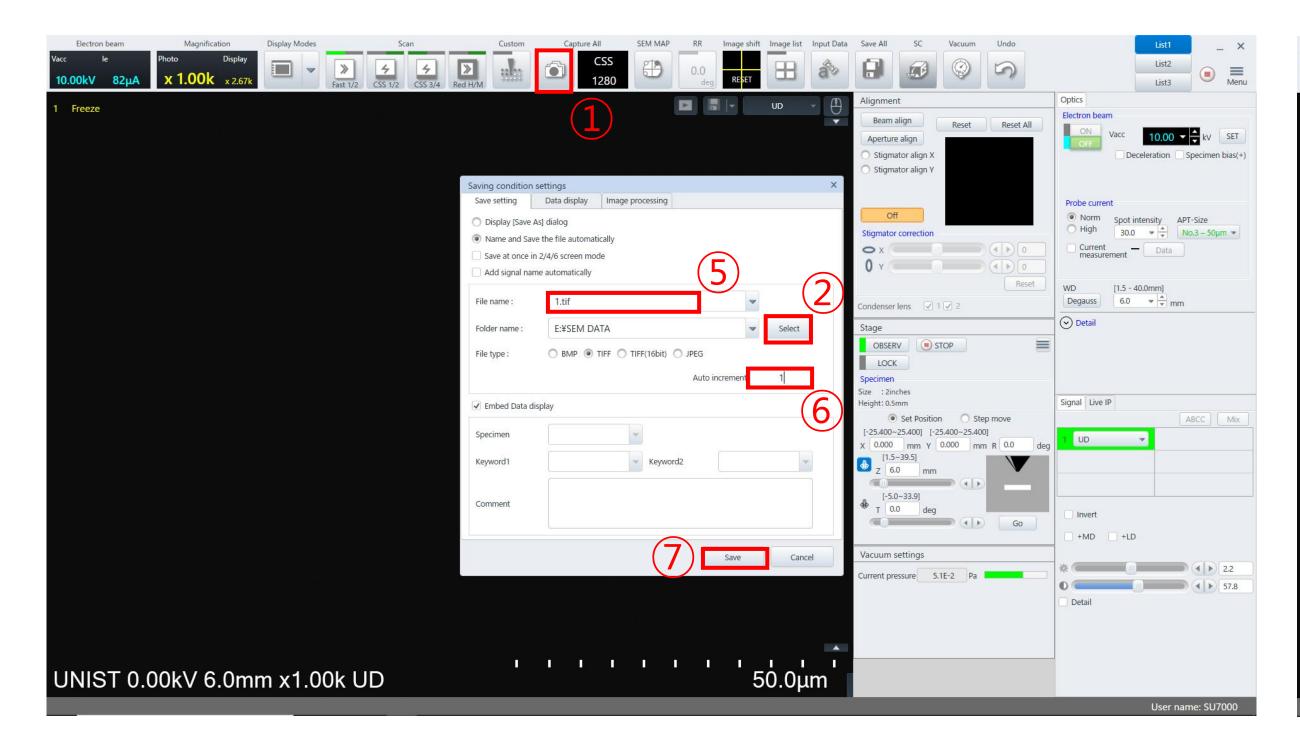

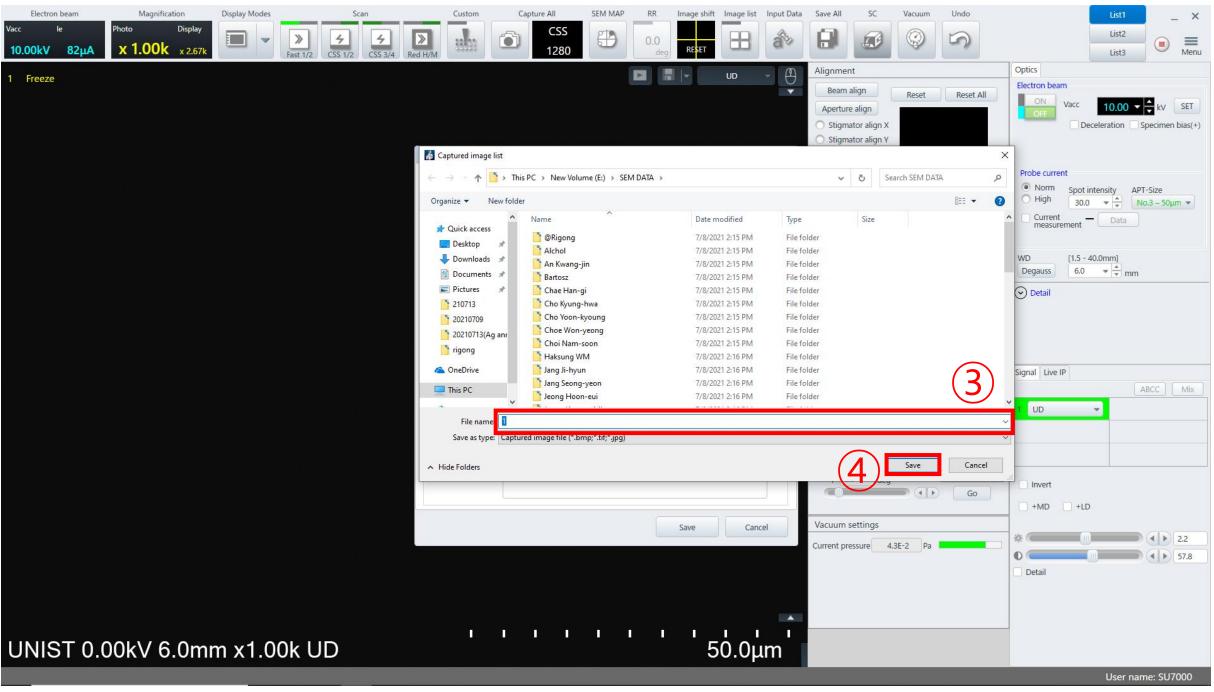


- 1. Right-click on [Capture All] [Capture] and click [Select].
- 2. Create a folder.(Desktop-SEM data-Analysis year-Professor folder-Personal folder-Date folder)
- 3. Enter a sample name in [File name] and click [Save].
- 4. Enter 1 in [Auto increment] and click [Save].

#### **Acceleration Voltage**

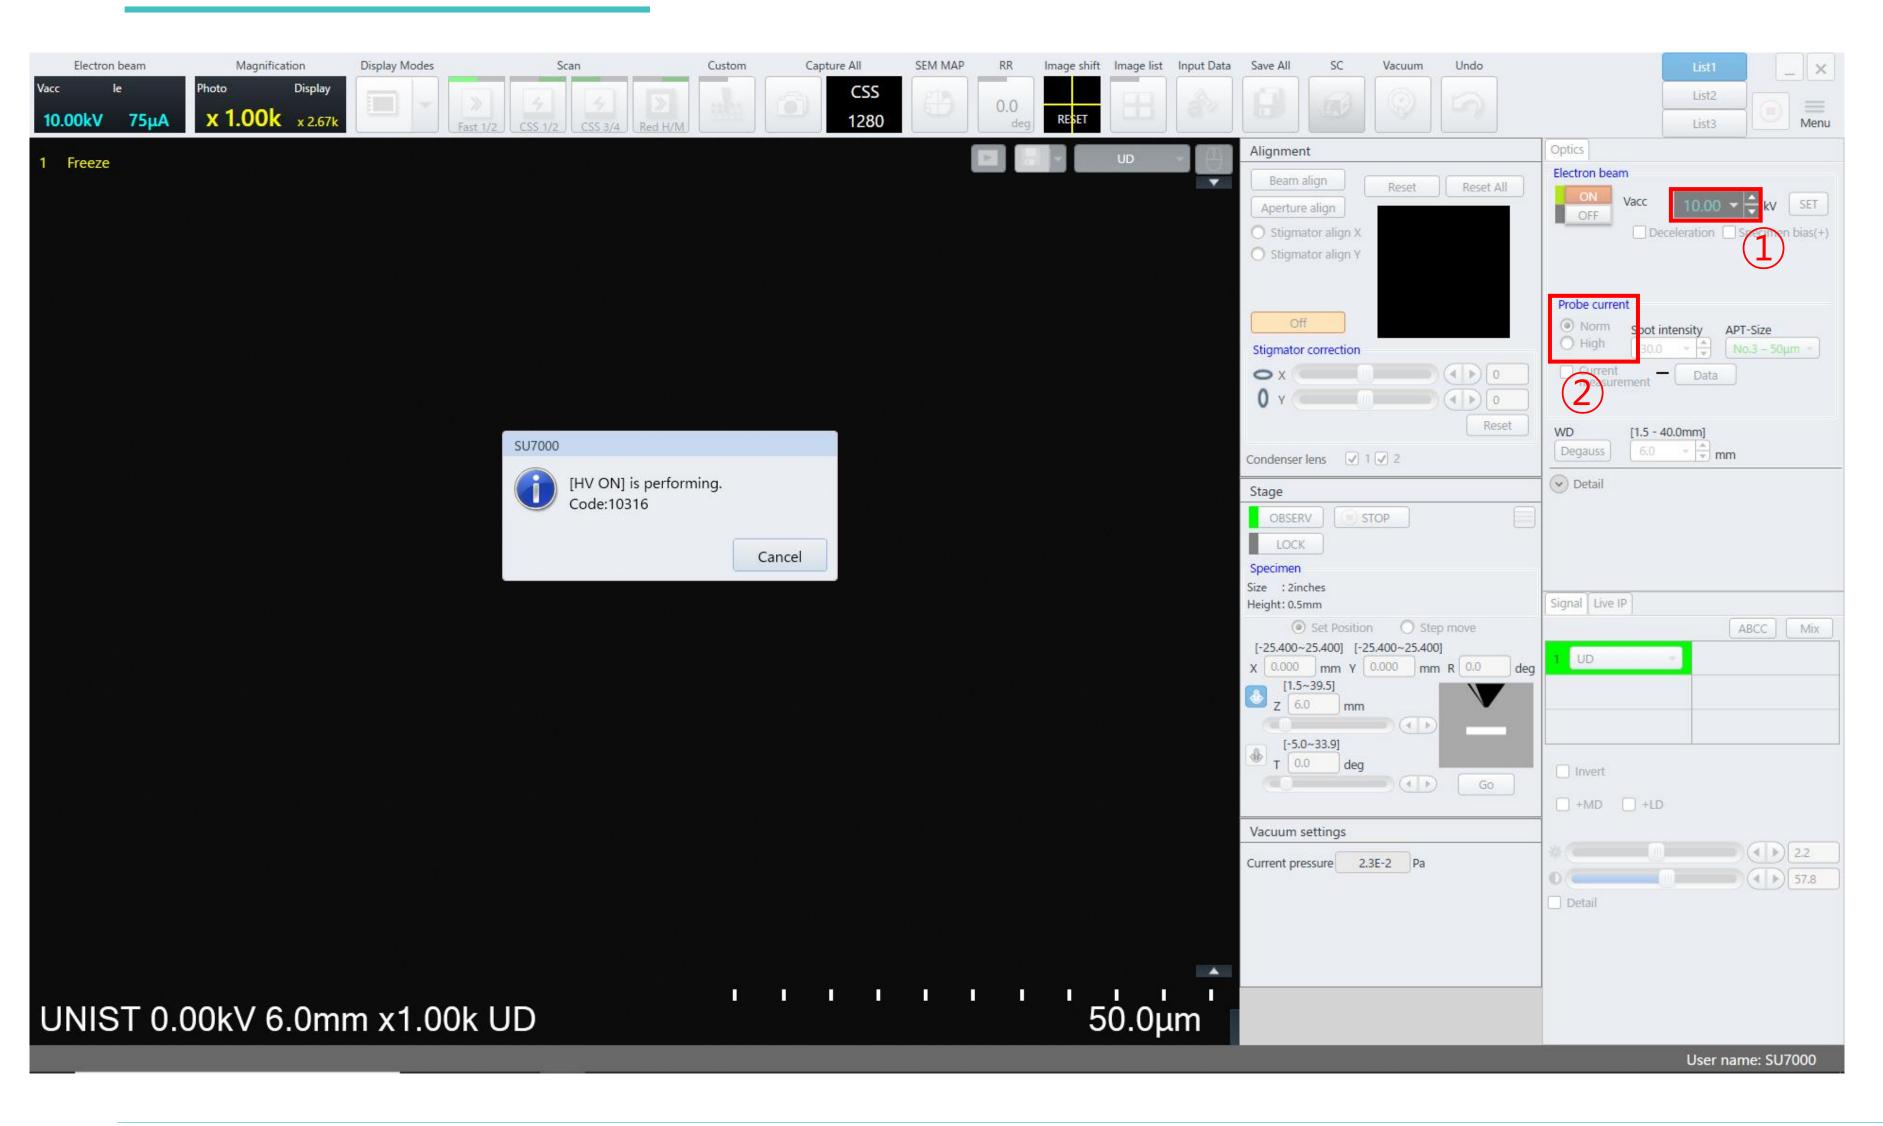

- Select the acceleration voltage in [Vacc].(5~10)
- 2. Select [Probe current] appropriately.


#### Beam on

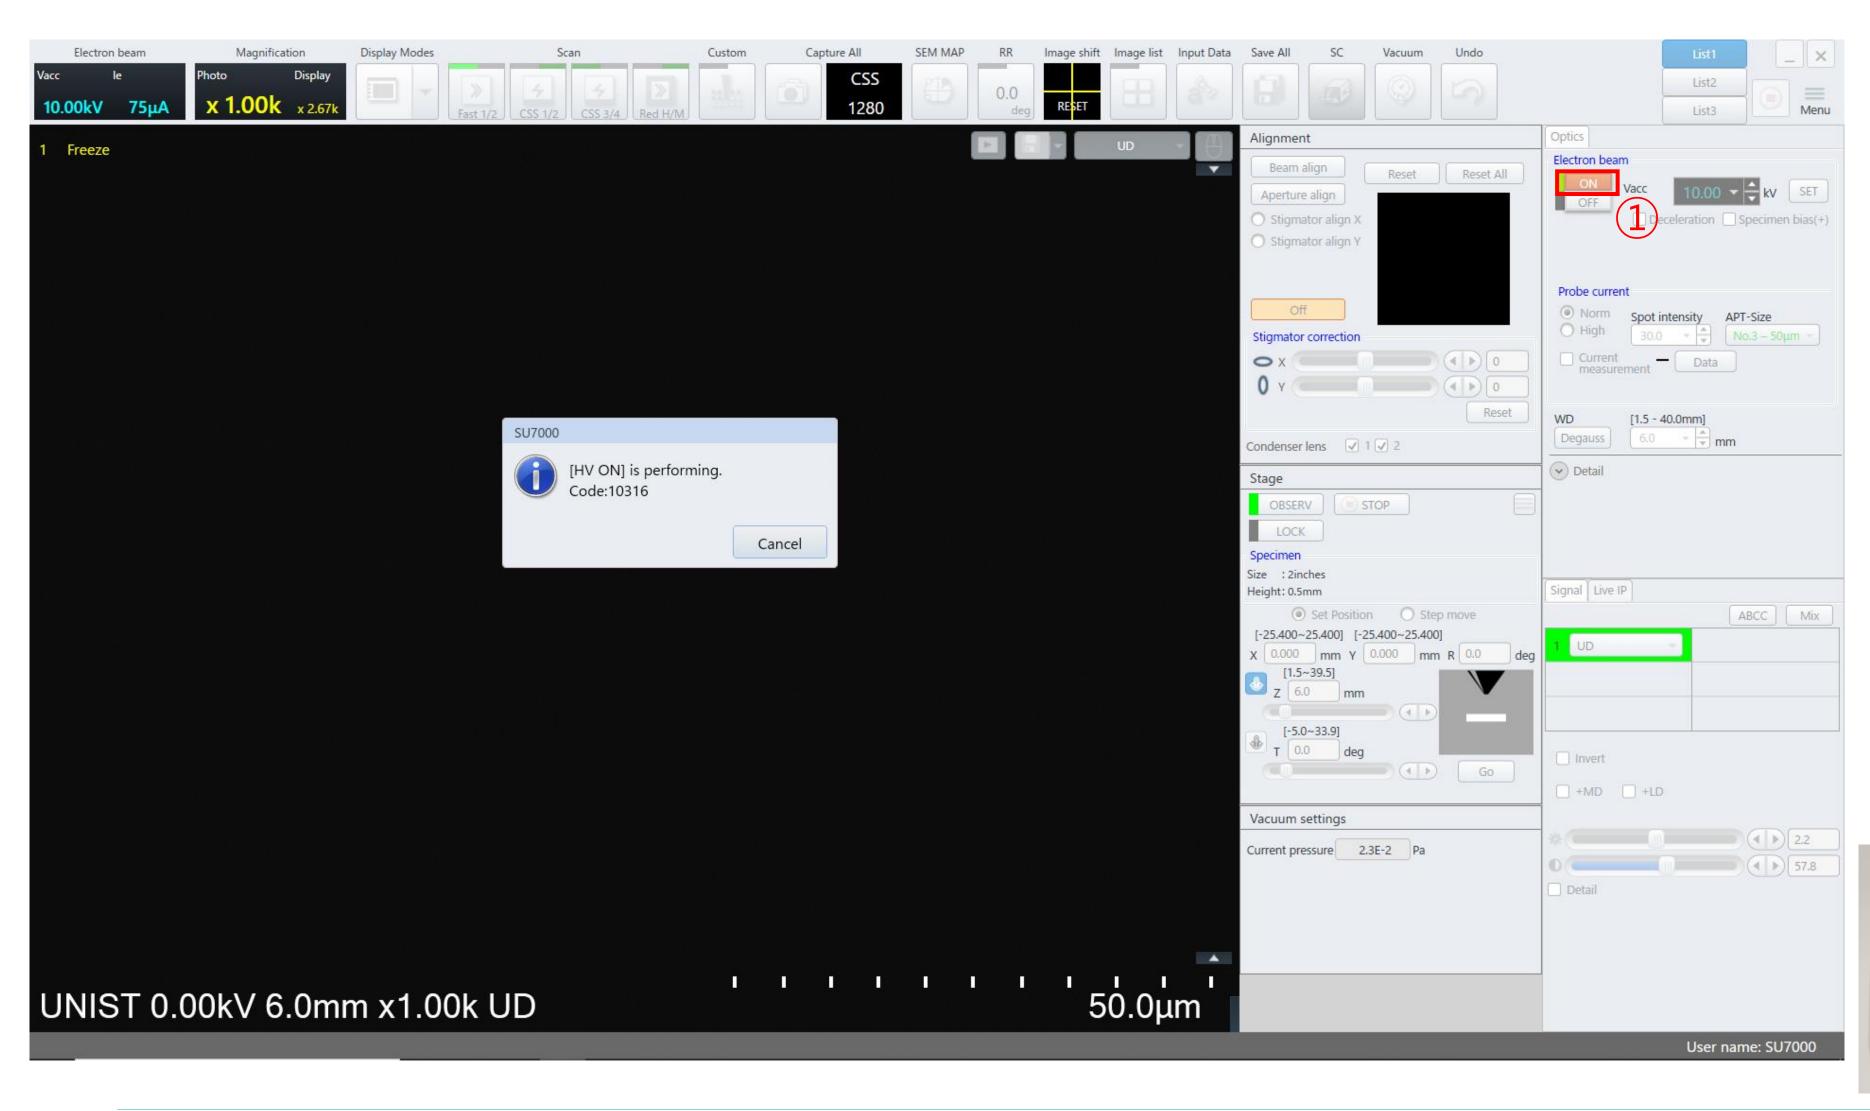


- 1. Click Electron beam [ON].
- If the screen is too dark or too bright, press [Auto].(You can manually adjust the [Brightness] or [Contrast] knob individually.) → This process can be performed at any time during image observation.




#### Finding the Specimen

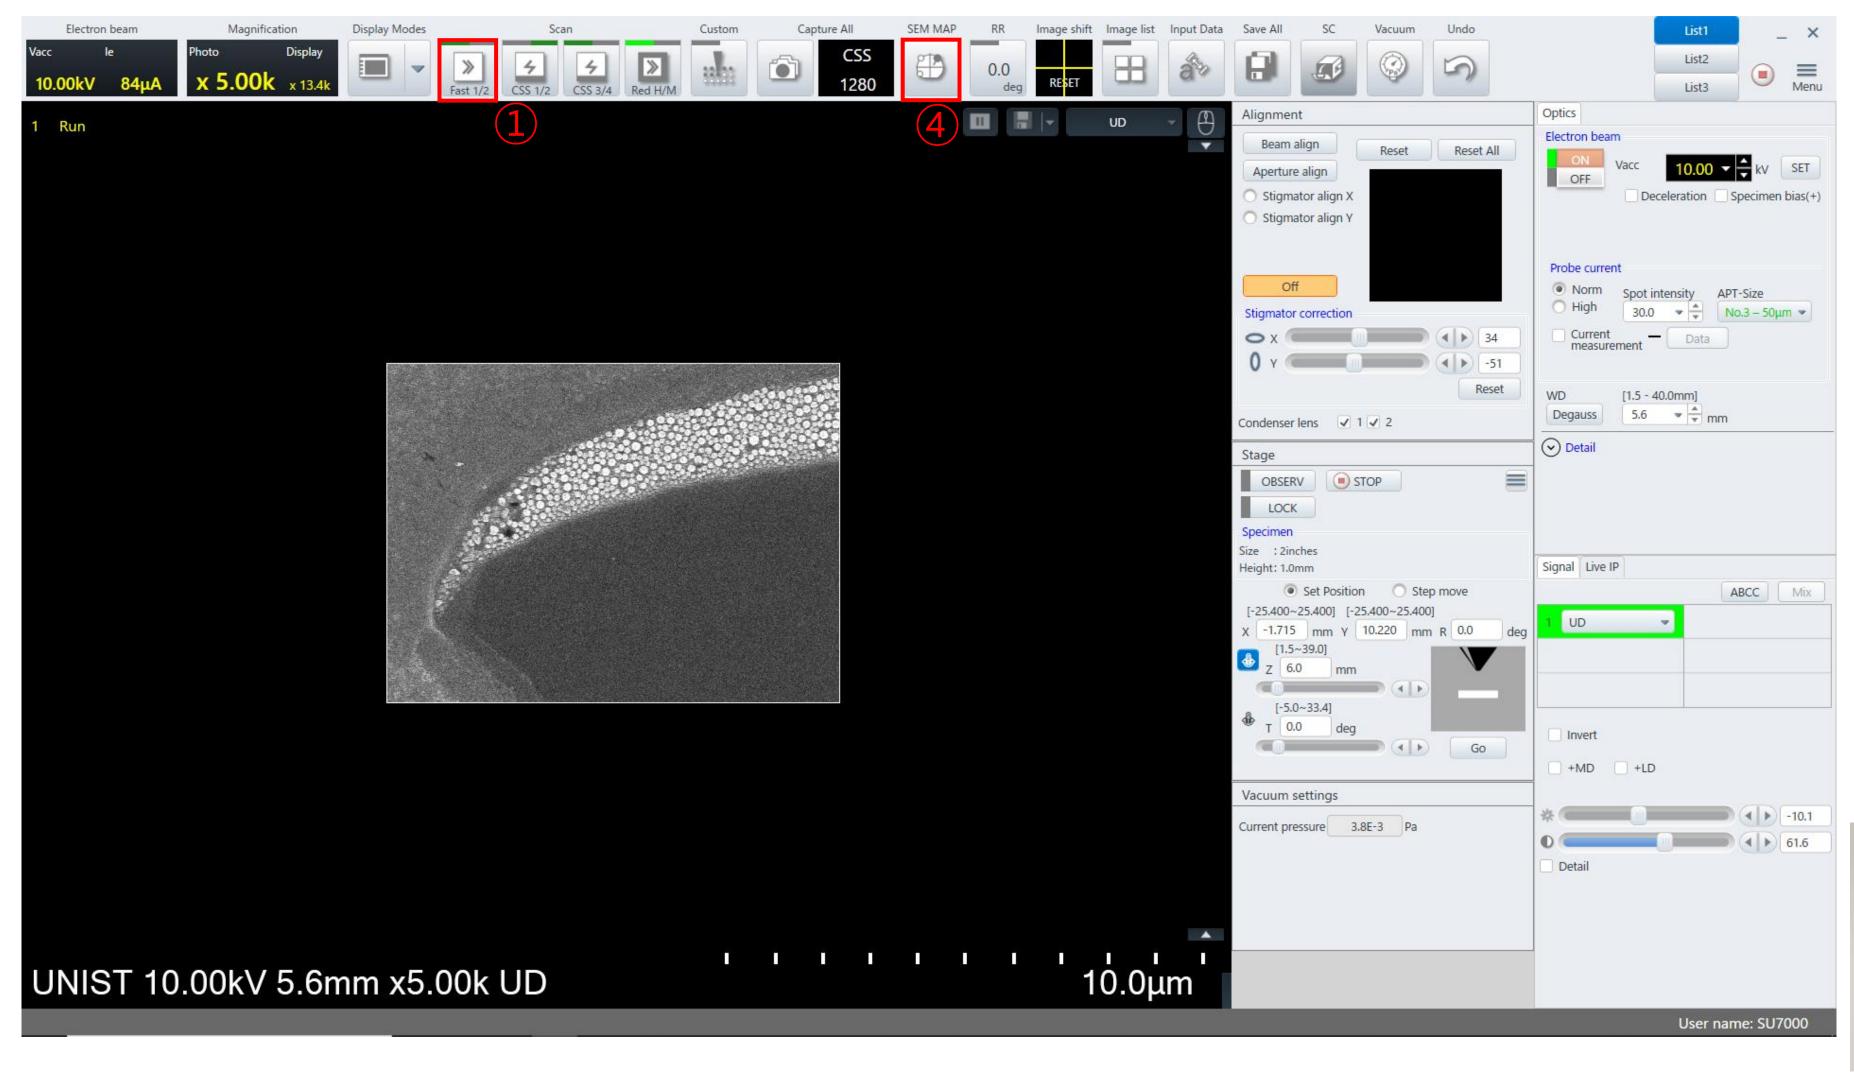

- Press the [SCAN 1](SCAN SPEED:SCAN1>SCAN2>SCAN3)
- 2. Press [LOW MAG]
- 3. If the image is blurry, use the focus knob to adjust the focus.

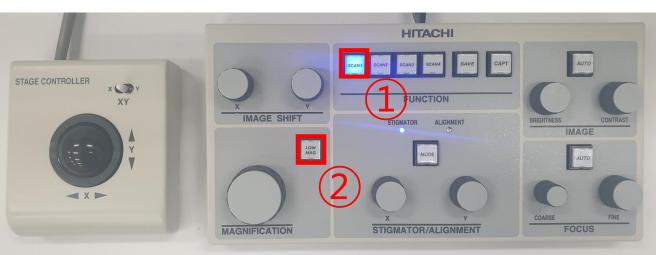

#### Finding the Specimen

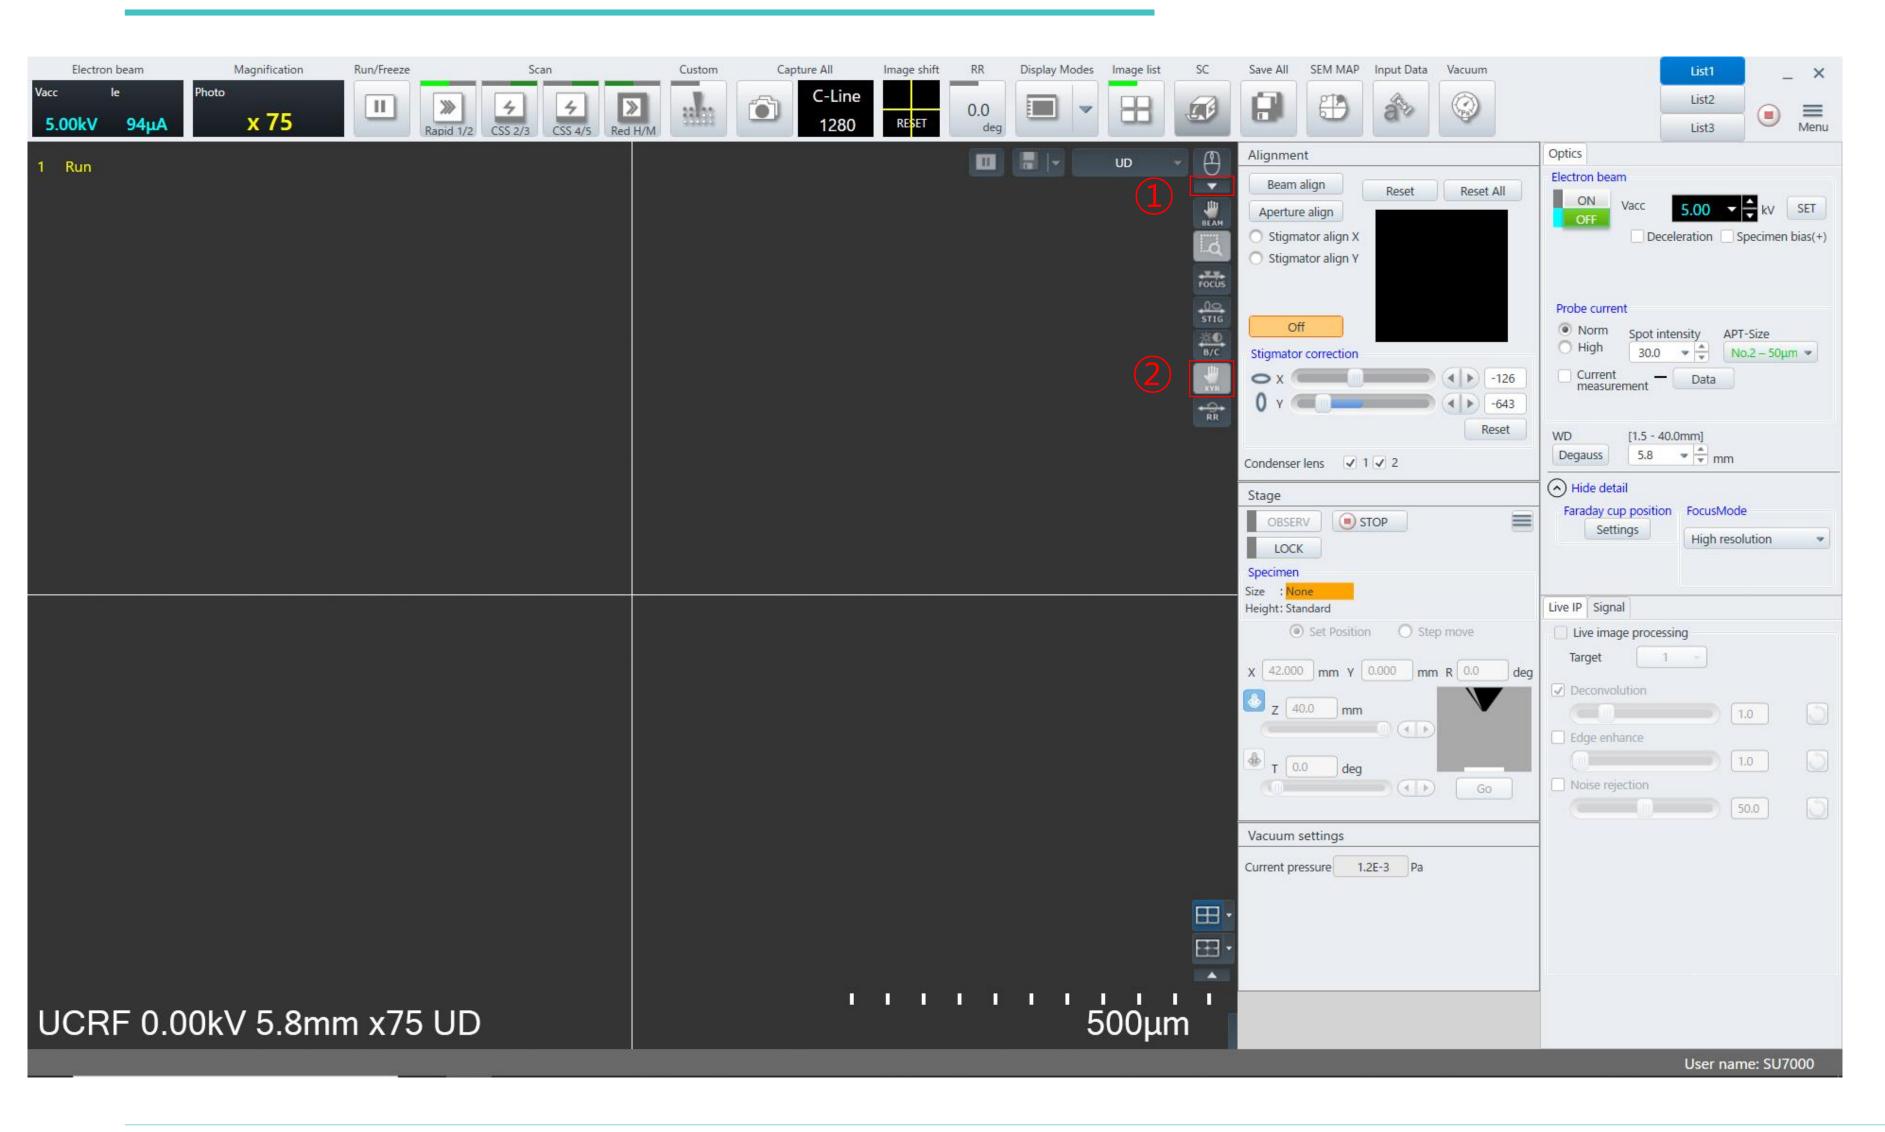

- 1. Click the mouse down arrow.
- 2. Press XYR.
- 3. The double-clicked location on the screen is moved to the center.
- 4. Please refrain from using the trackball as much as possible.(wear and tear issues)


#### **Focus**




- Move the stage to the location you want to observe.
- 2. Use the magnification knob to slowly raise the magnification to 5000 times and adjust the focus in between.
- Coarse: fast adjustment
- Fine: fine adjustment




## **Stigmator**

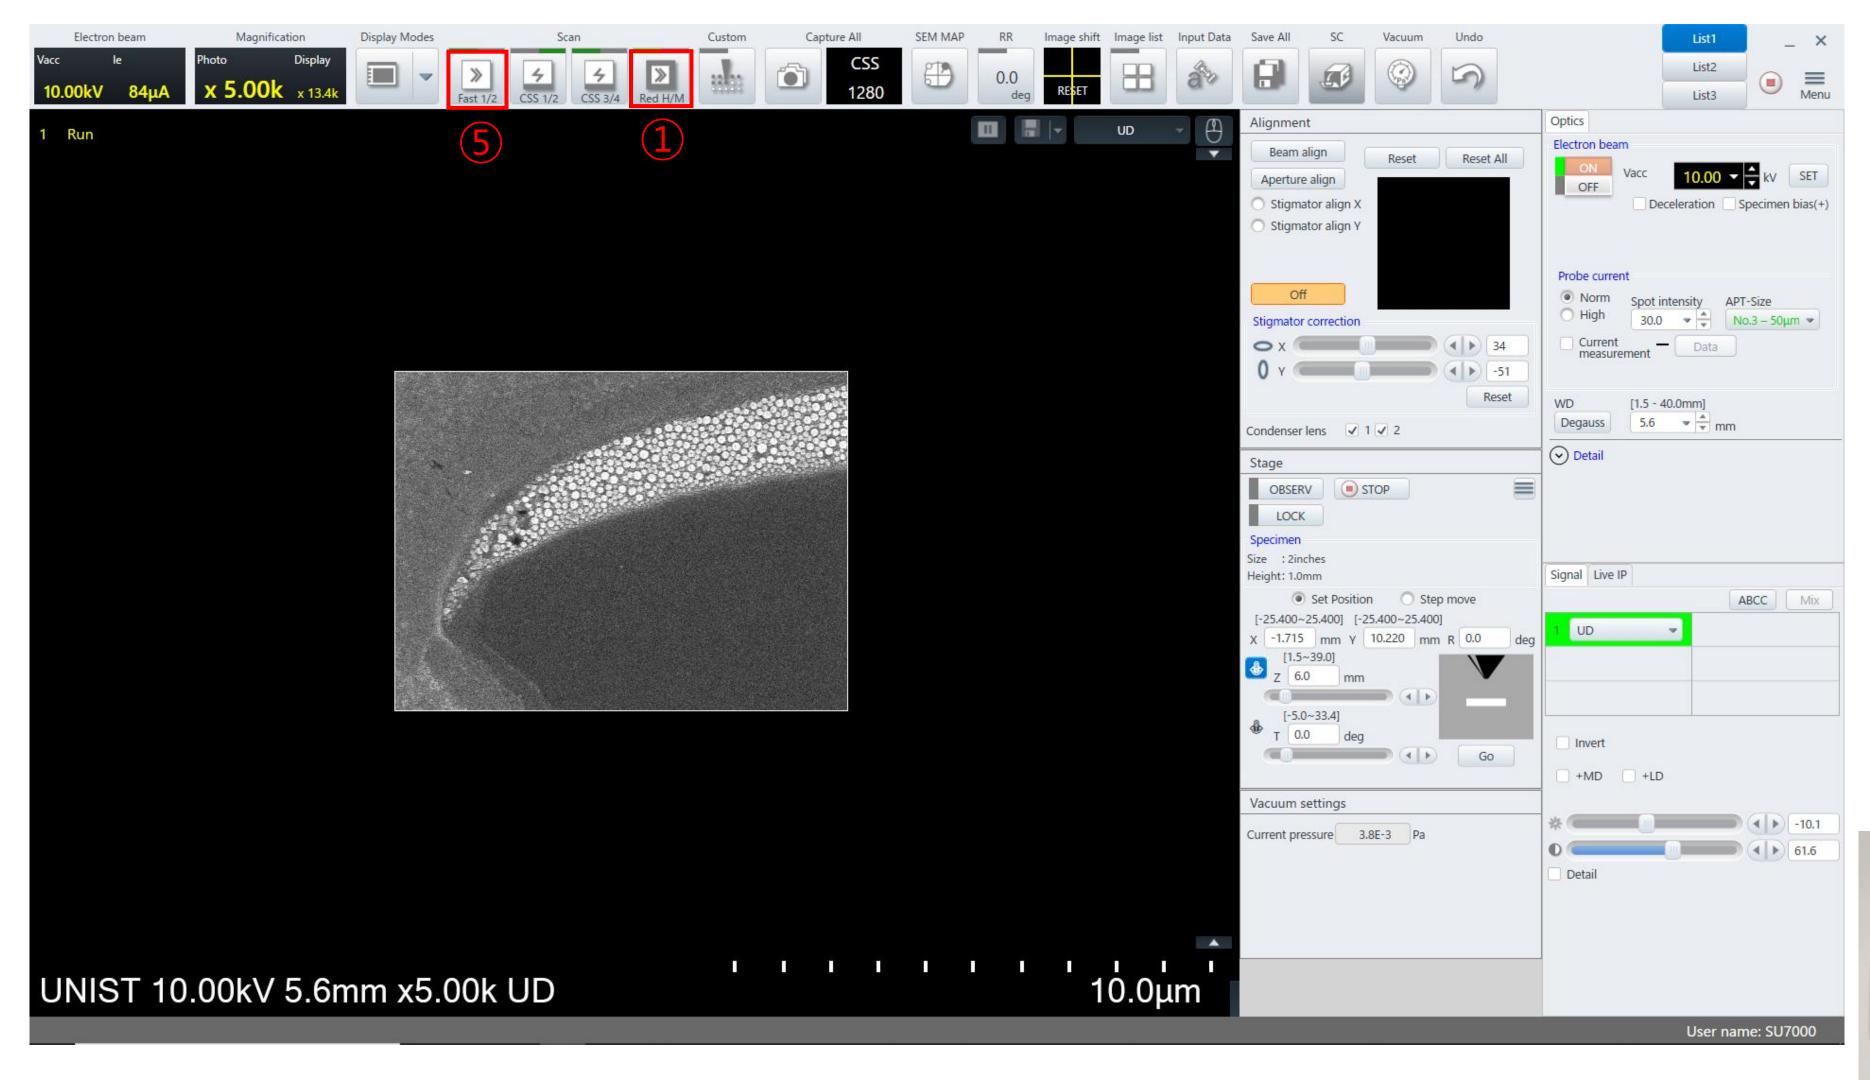

- 1. Press [SCAN 4].
- 2. Adjust the focus.
- 3. Adjust the Stigma X and Y knobs one by one.
- 4. Adjust the focus.
- 5. Press [SCAN 1].

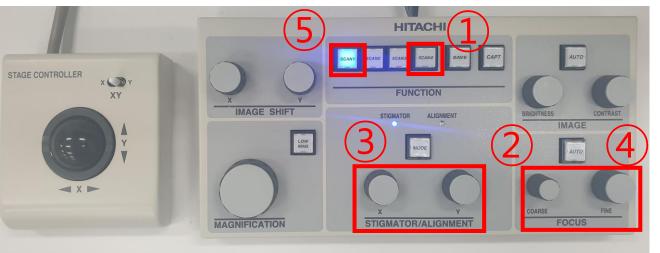

#### Working distance

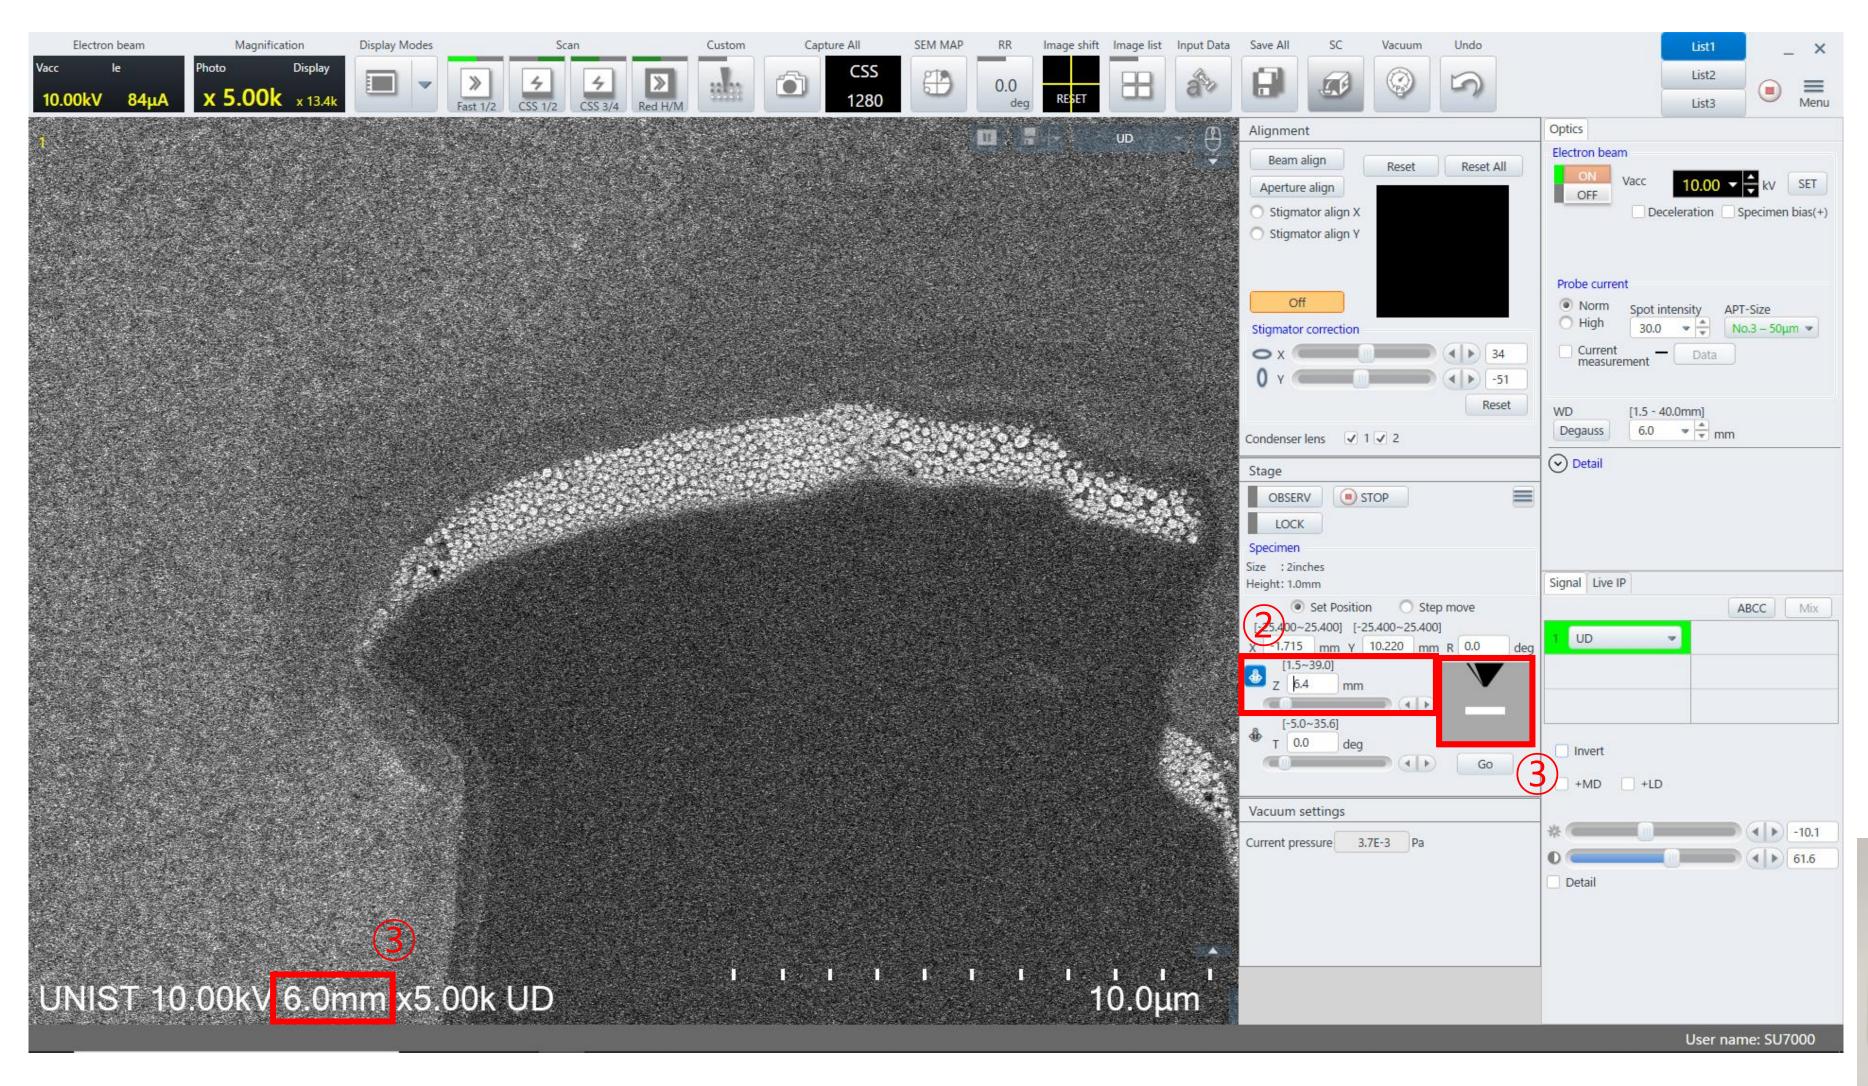


- Check WD at the bottom of the screen
- Subtract the WD found in 6, and subtract that
   value from the [Z] value.
- 3. Enter the calculated value in [Z].
- 4. Click [Move].
- 5. Adjust the focus.






#### **Beam Alignment**

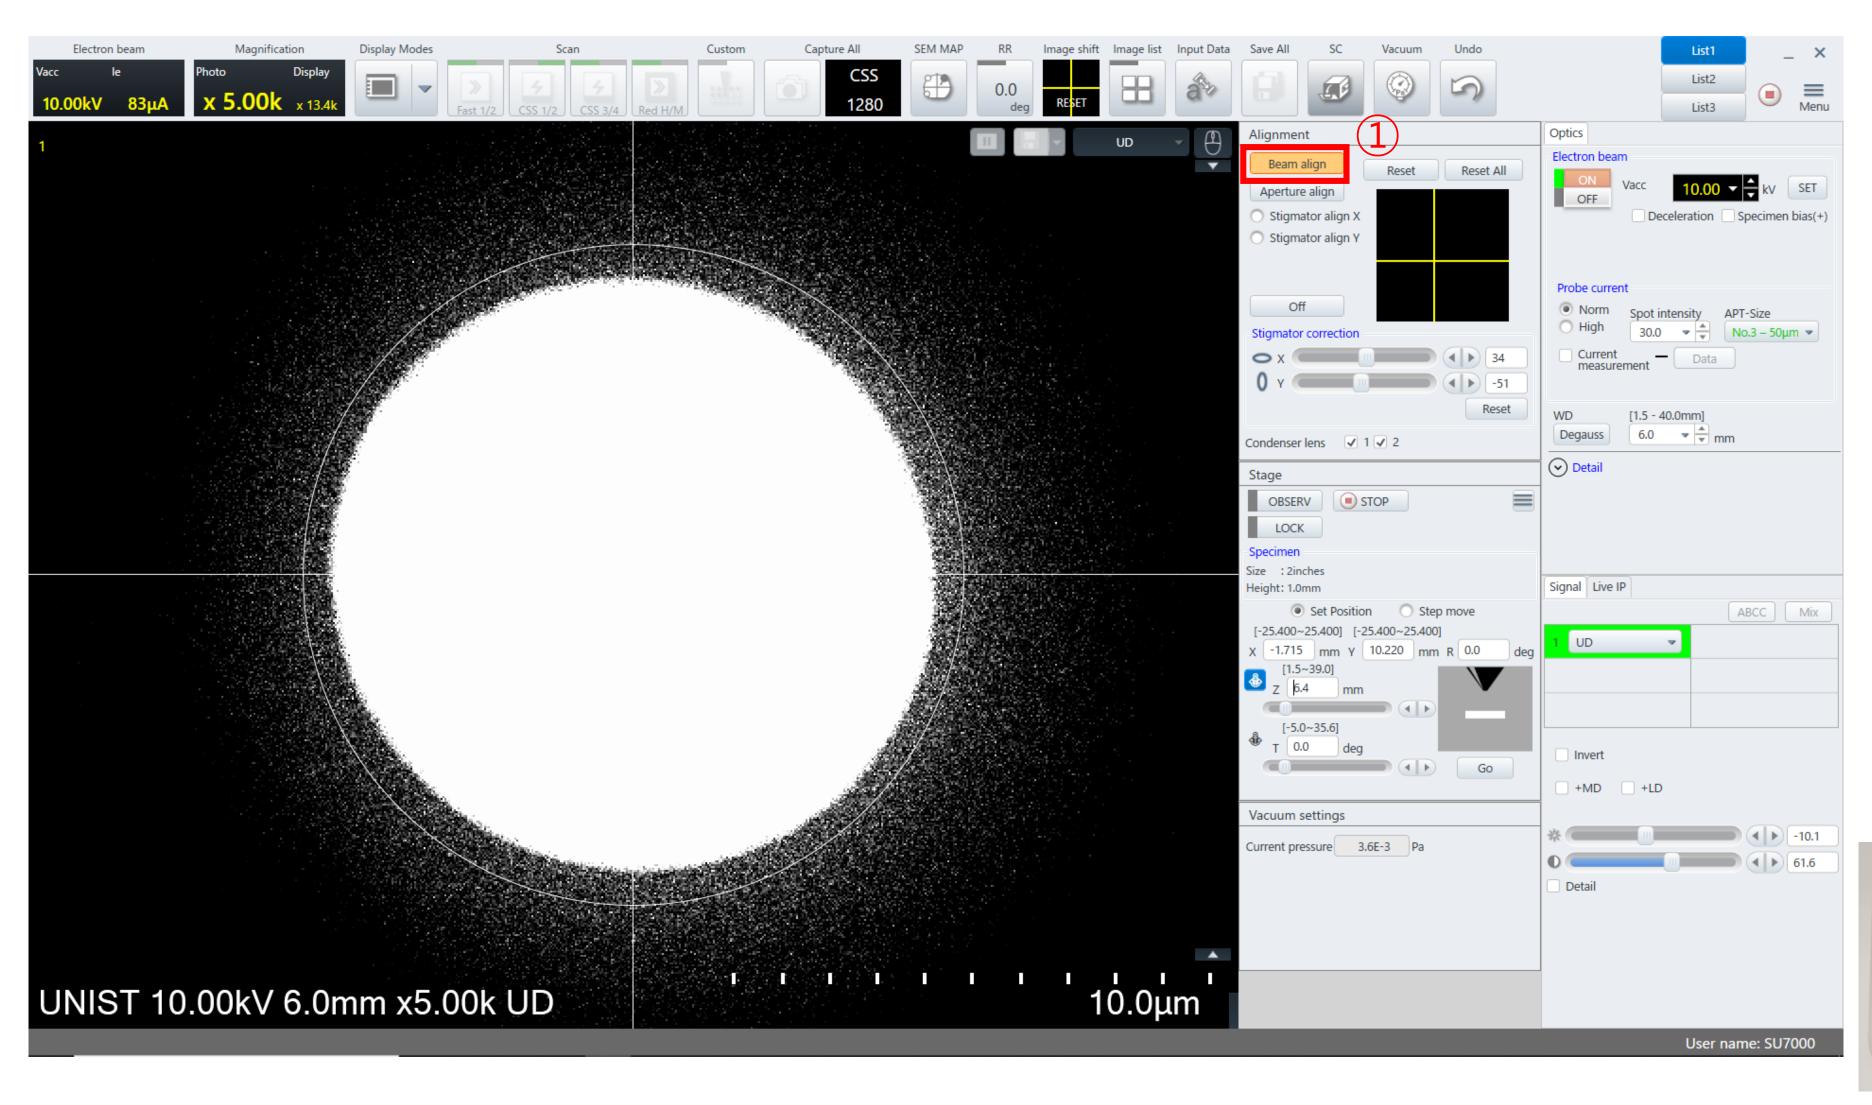


- 1. Press [MODE].
- Adjust the STIGMA X
   and Y knobs one by
   one to bring the beam
   to the center.
- 3. Press [MODE].

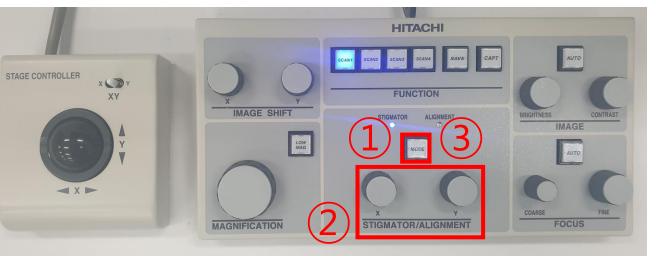


#### **Beam Alignment**



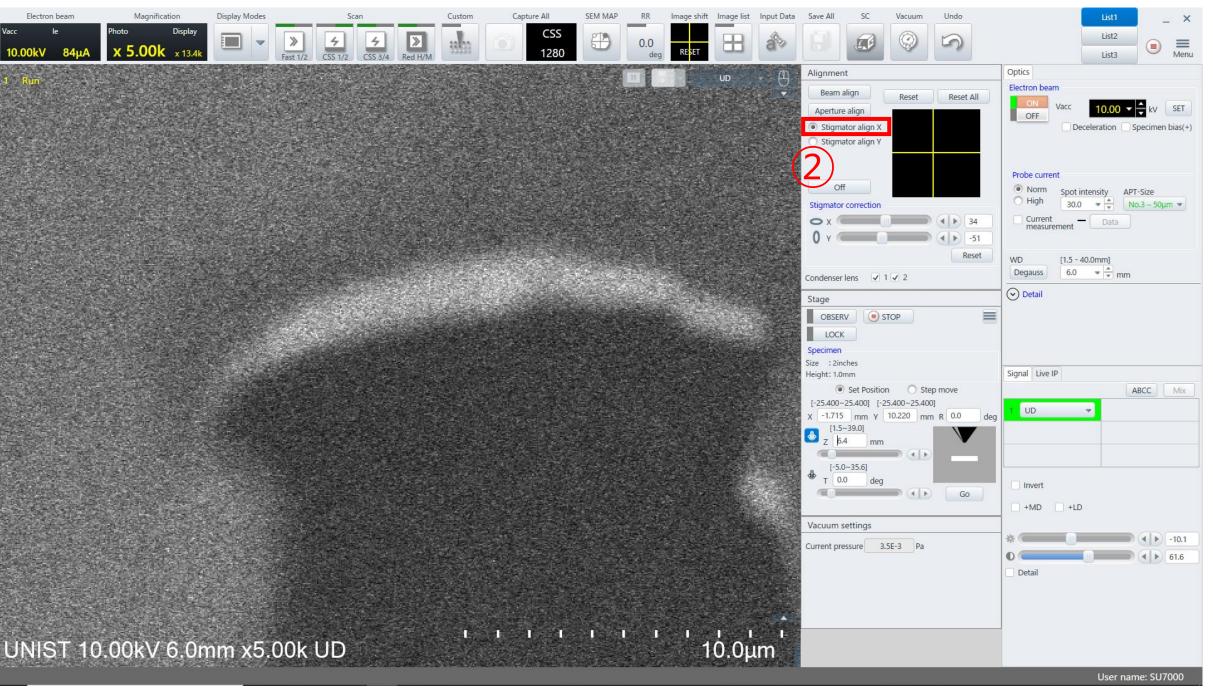

- Check [Cross maker]. And adjust the stigma X and Y knobs one by one so that the specimen moves in place.(STIGMA X: ↔, STIGMA Y: ‡)
- 2. Press [MODE]. And adjust the stigma X and Y knobs one by one so that the specimen moves in place.(STIGMA X:  $\nwarrow \searrow$ , STIGMA Y:  $\nearrow \swarrow$ )


#### **Beam Alignment**

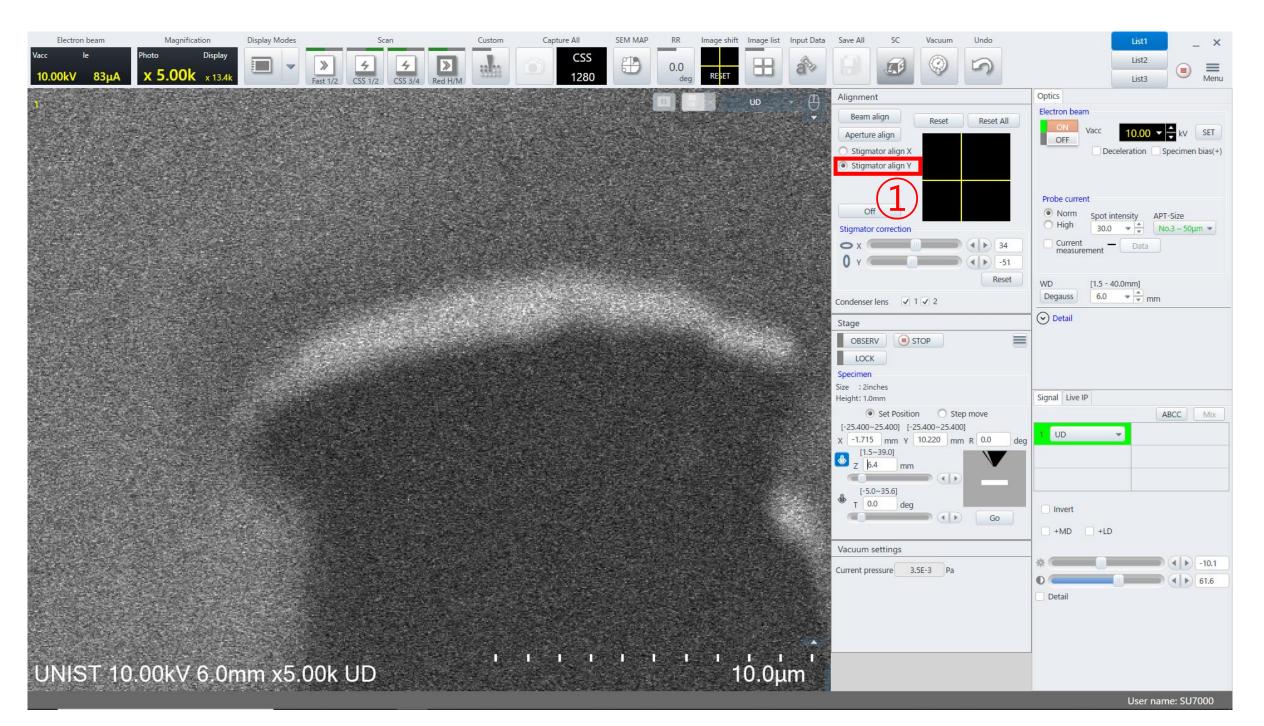



- 1. Press [MODE].
- 2. Adjust the stigma X and Y knobs one by one so that the specimen moves in place.(STIGMA X: ↖ ↘, STIGMA Y: ↗ ∠)
- 3. Press [MODE].


#### Saving the Image

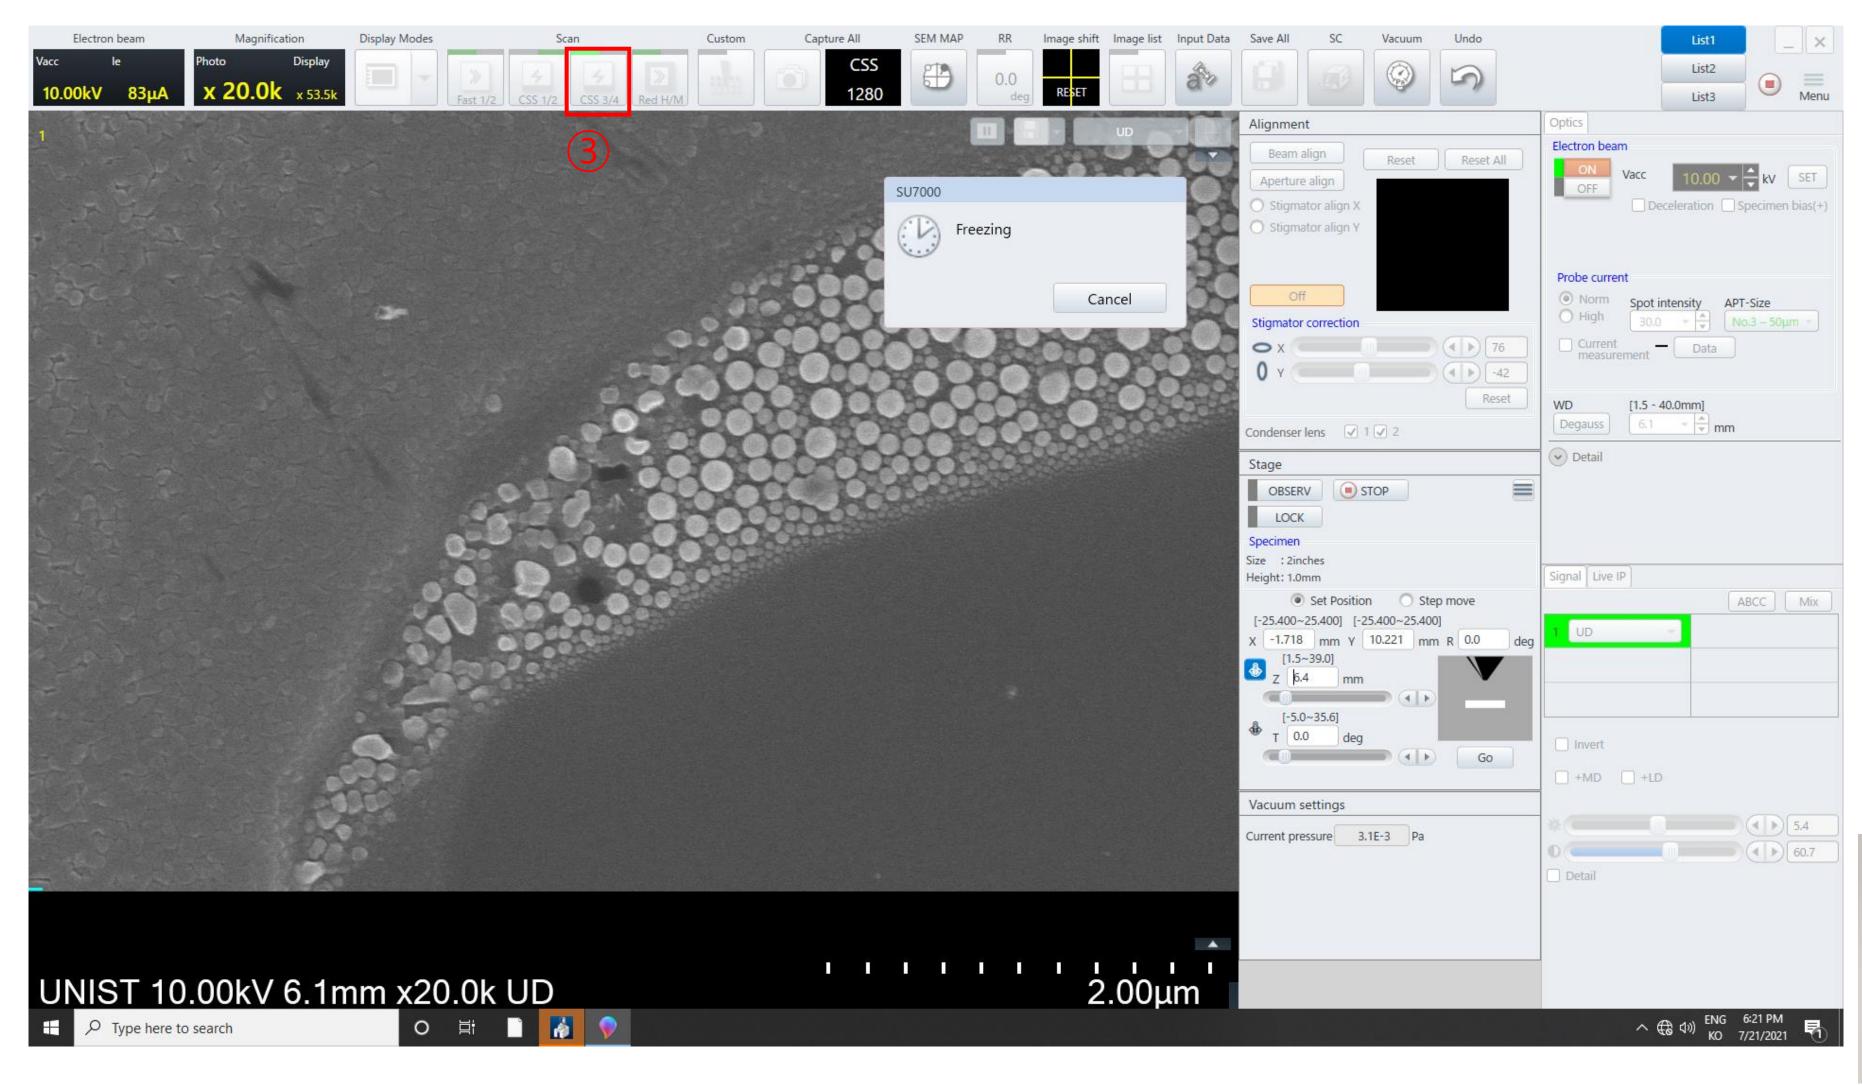


- Move to the location you want to observe.
- Adjust the magnification slightly higher than the magnification you want to observe.
- 3. Click [SCAN 4].
- 4. Adjust the knobs

  [FOCUS]-[STIGMA X,


  Y]-[FOCUS].

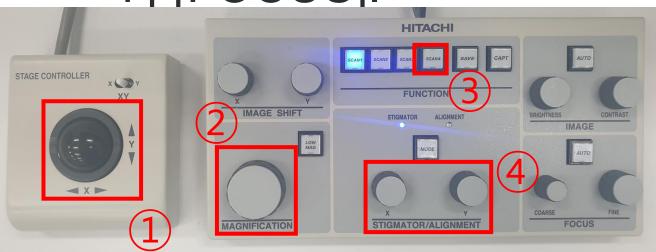


## Saving the Image

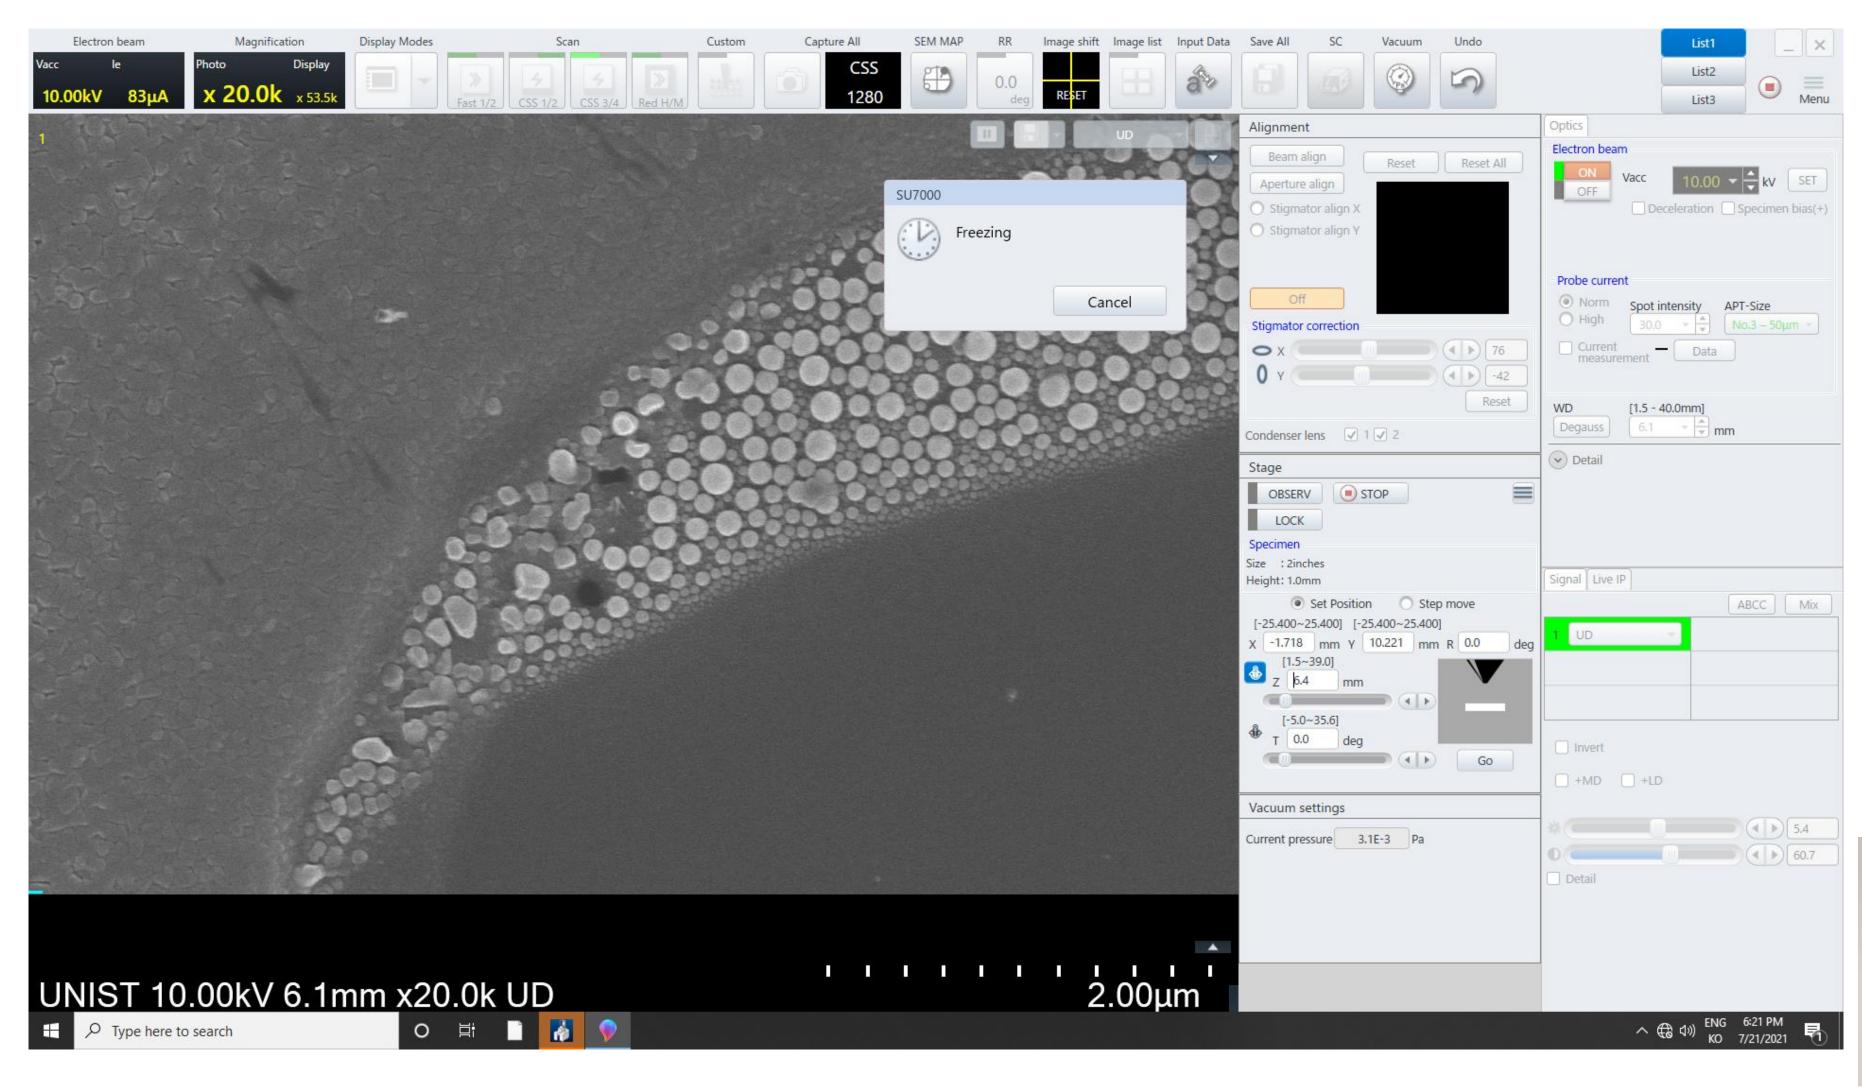


- 1. Click [SCAN 1].
- 2. Adjust to the desired magnification.
- 3. Press [SCAN 3] -[SAVE] or [CAPT].
- 4. Press [SCAN 1].
- 5. Repeat steps 1 in the previous slide to 5 in this slide.

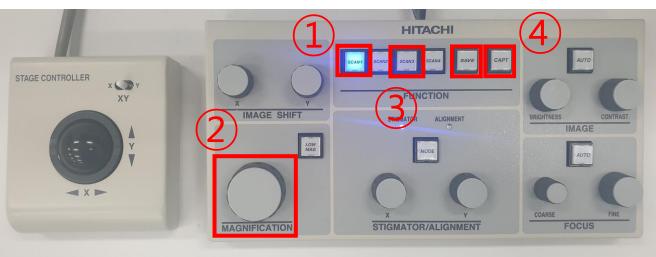


#### **Finish**

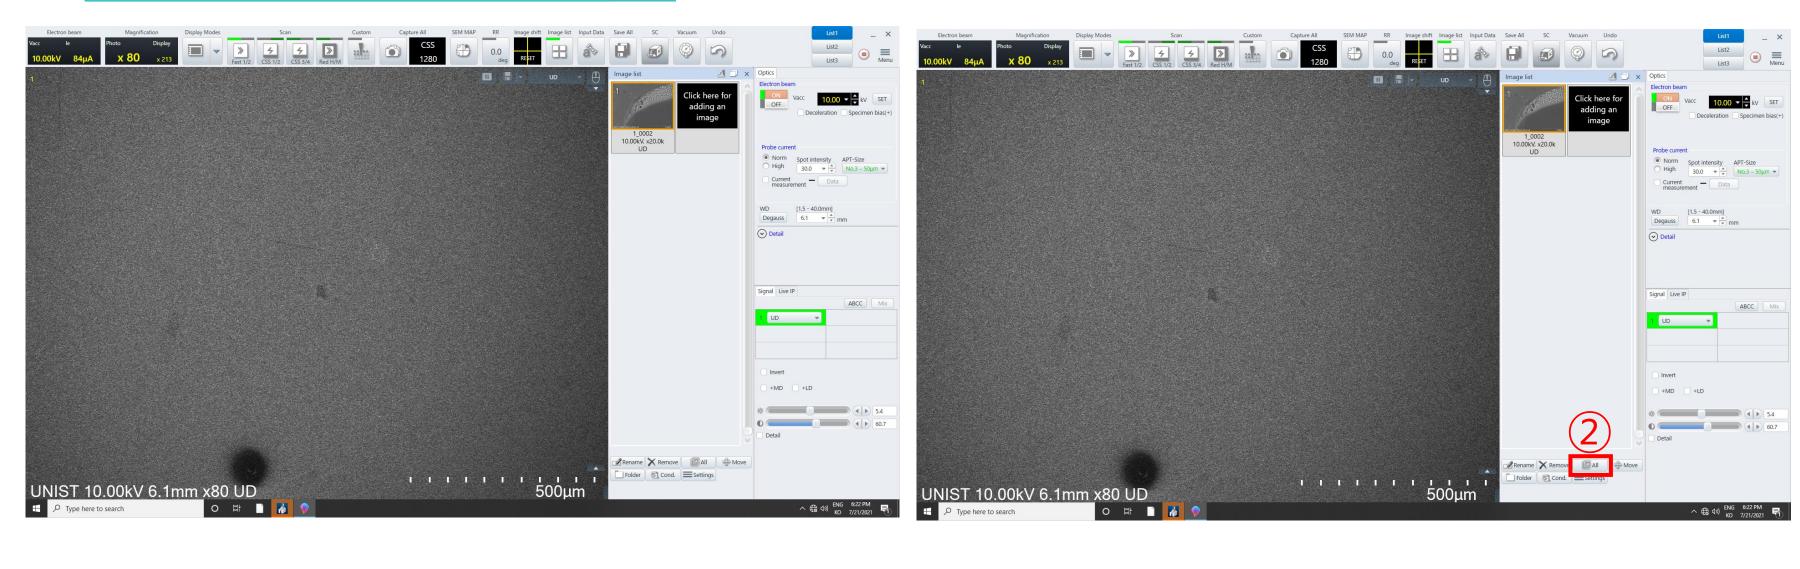


1. Press [LOW MAG].

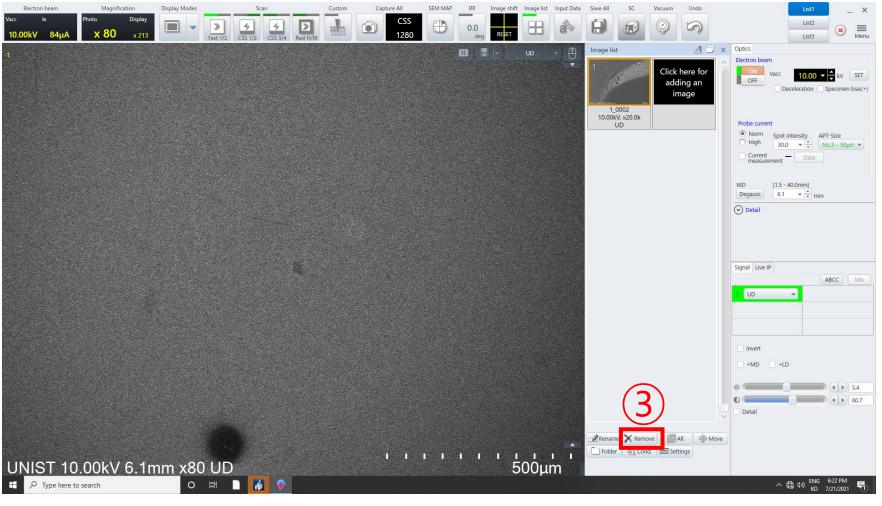


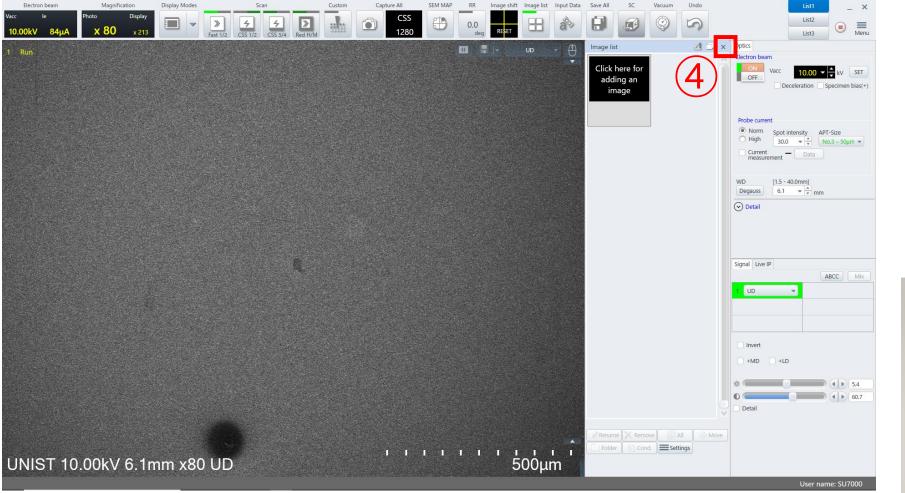




#### **Finish**

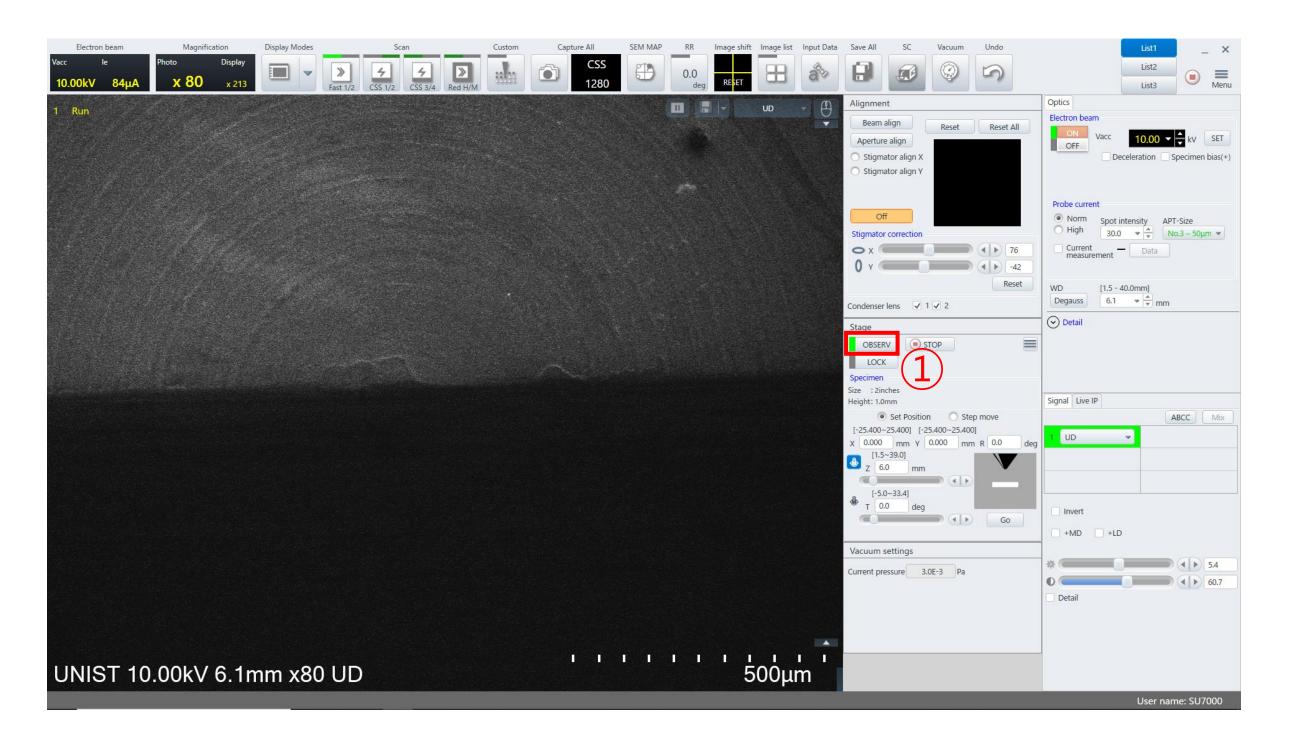


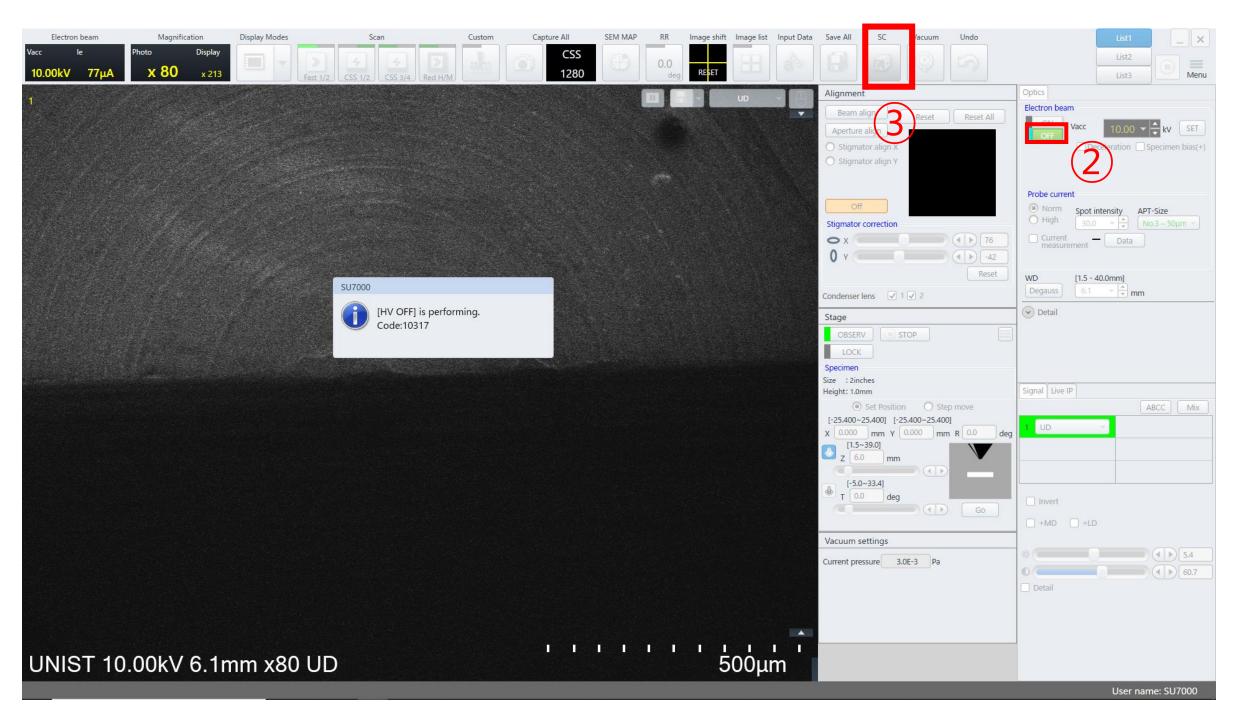

- 1. Click [OBSERV].
- 2. Wait until the green light stops blinking.★
- 3. Click Electron beam [OFF].★
- 4. Click [SC] [Air].


# Retrieving the holder

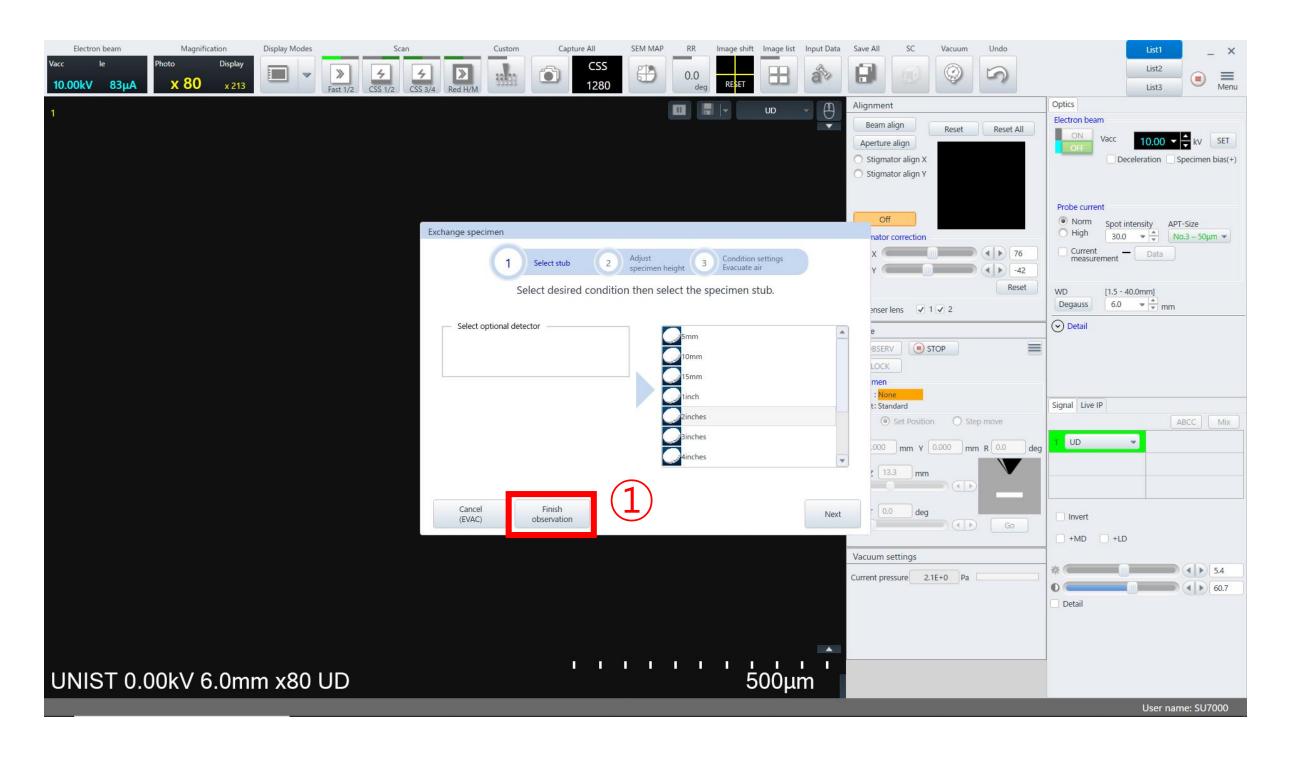

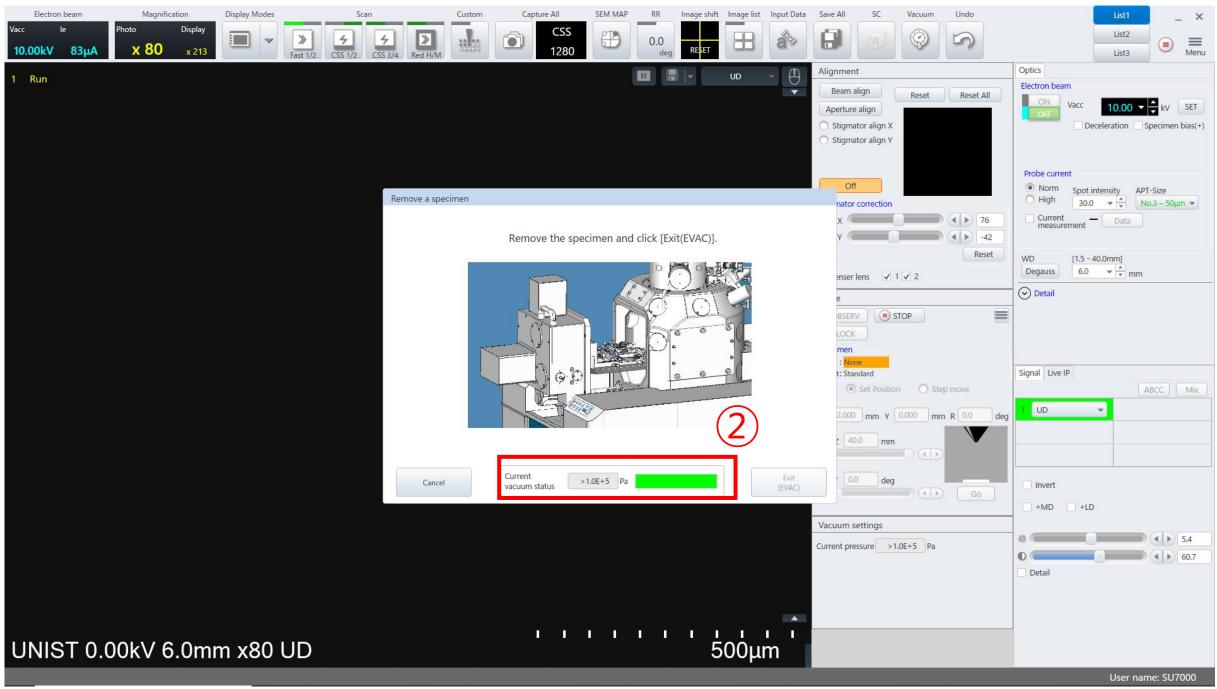

- 1. Click [Finish observation].
- 2. Check the vacuum and remove the specimen.
- 3. Click [Exit(EVAC)].
- 4. Click [OK].

#### **Transfer SEM data**

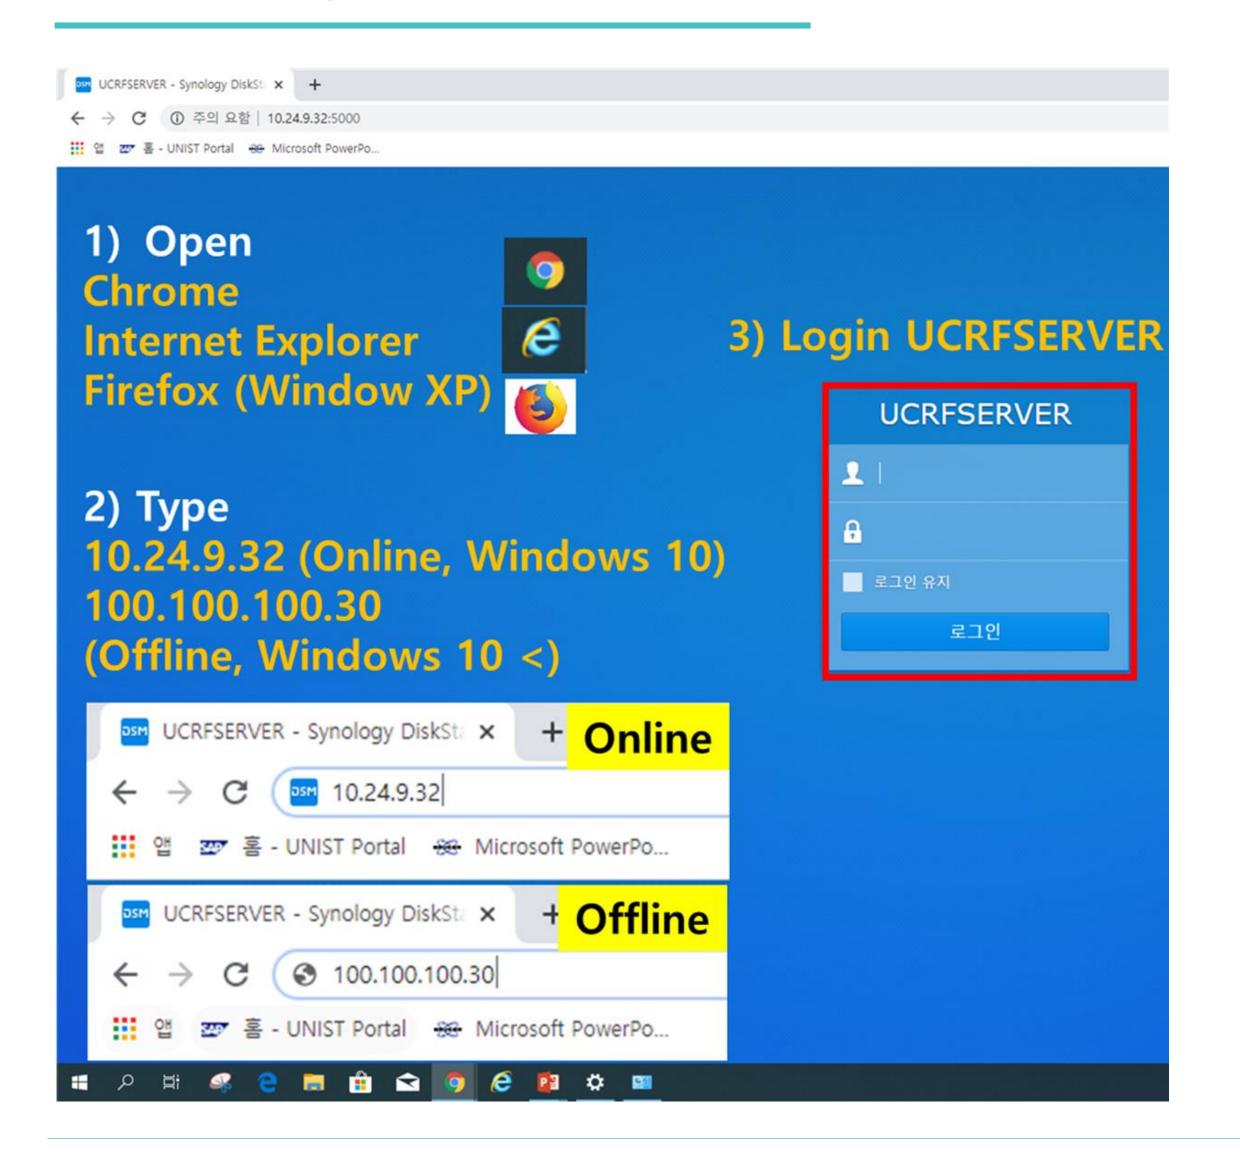

- 1. Do not use USB when transferring SEM data.
- 2. Double-click the web browser.(Chrome, etc..)
- 3. Enter 100.100.100.30. in the address bar.(Enter 10.24.9.32 when downloading from Lab)
- 4. Enter your Lab ID and password.
- 5. Find your professor's folder and create your own folder.
- 6. Drag the SEM data into your own folder.
- 7. Close the window when the move is complete.
- UCRF server manager: Park Ji-hye(052-217-4035)

#### Daily Checklist in the lab

- 1. Put the specimen holder back in place.★
- When using weekends or holidays, check the [Daily checklist in lab] and sign the checker's signature.
- Enter the name of your advisor and submit it in the original place with your signature or stamp.★


#### Daily checklist in lab.

Lab title	Electron Microscopy Preparation	Bldg./NO.	102-B115	Date			
Division	vision checkpoint					check	
	Laboratory overall cleanliness condition.						
	Smoking or bringing food into the lab.						
General Safety	Management status of experimental equipment such as safety regulations, safety signs, personal protective equipment, first aid, etc.						
	Checking the pr	Checking the presence of a pre-hazard risk analysis report.					
	Checking the power supply status of unused electrical equipment and checking for overloaded outlets.						
Electric		Using grounded outlets, checking damage on the insulating coating of electric wiring, electric wiring arrangement.					
		Checking ground conditions for preventing external or static disturbances of the instrument.					
	Non-load statu	Non-load status around electric panelboards.					
	Fire extinguisher sign, proper fire extinguisher and regular inspection status.						
Fire	Emergency exits, escape routes, and any obstacle blocking the passage.						
	Storage of foreign substances around fire hydrant and fire extinguishers.						
		ge of gas cor ventilation con		isk of t	ipping over,		
	Corrosion, deformation, nozzle lock status on the exterior of the gas containers and checking the packing time limit of gas containers.						
Gas	Checking installation and operational status of gas leakage detection alarm, anti-backflow/anti-backfire prevention devices, neutralizing decontamination devices.						
	Attachment of pipe marks, gas facility boundaries/warning marks and operation status of regulators and valves.						
	Safe separatio	paration distance from surrounding fire hazards.					
	Keeping hazardous factors handling and management registers and MSDS.						
Chemical	Categorizing chemicals by description and storing chemical reagents in safety cabinets.						
Equipment check SU8220 Cold FE-SEM user: Check the pressure of nitrogen gas							
Confirm		Inspector	Signature			(sign)	
Col		Lab Director	Signature			(sign)	




## If you encounter a problem while using SEM 1

- How to reboot SEM and PC
  - 1. Beam off
  - 2. Close the SU7000 program
  - 3. Shutdown the PC
  - 4. Off the EOC power
  - 5. After 10s, turn on the EOC power
  - 6. Turn on the PC
  - 7. Open the SU7000 program
- If the sample keeps moving
  - 1. Because the specimen is not completely fixed
  - Charge up phenomenon → Need to lower the acceleration voltage or add more coating

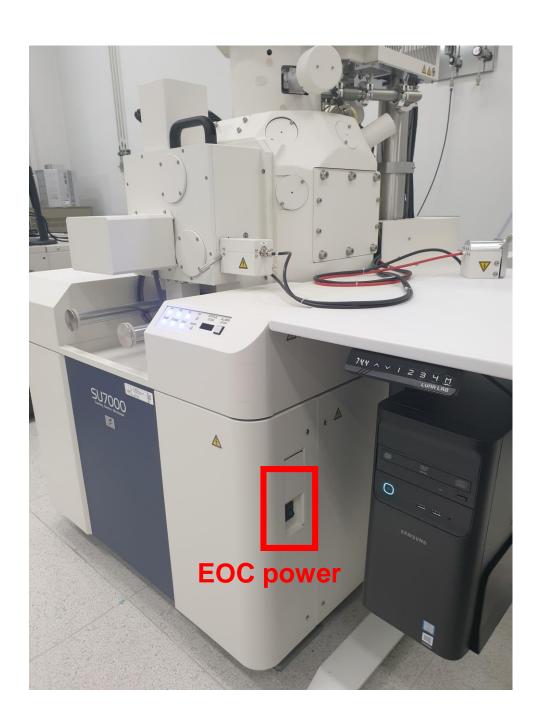


#### If you encounter a problem while using SEM 2

EDS connection problem 1

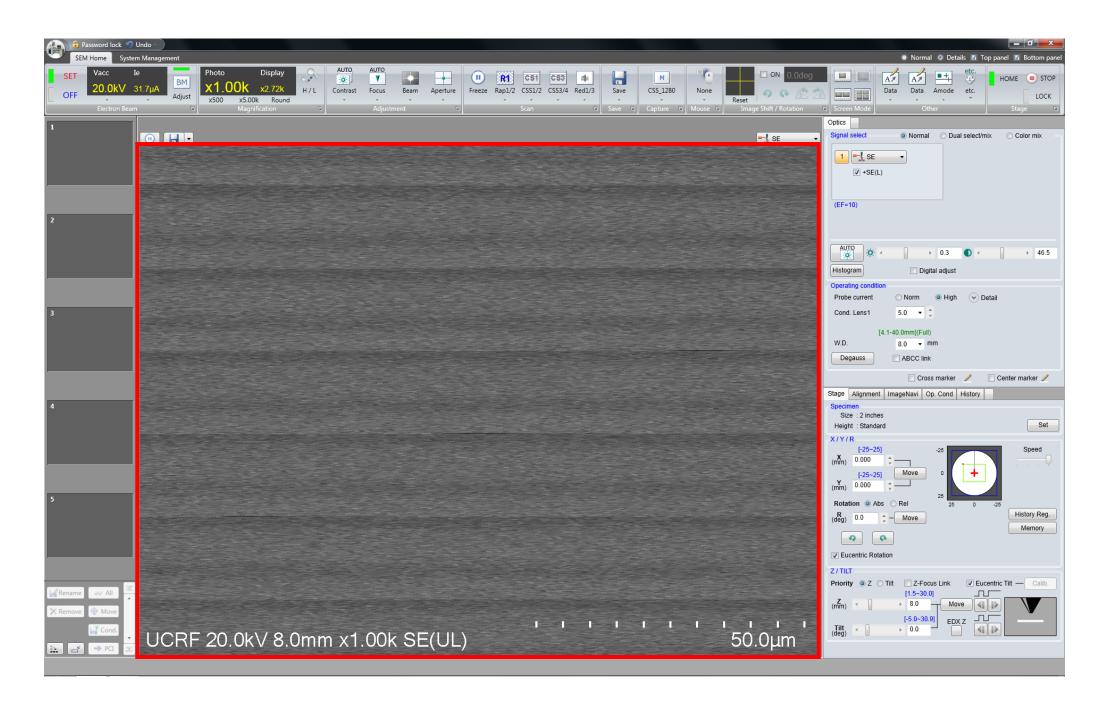

- If the SEM screen is bad
   (Beam alignment is also not possible)
  - Reboot EDS PC(PW: ucrfumcl1!)

EDS connection problem 2

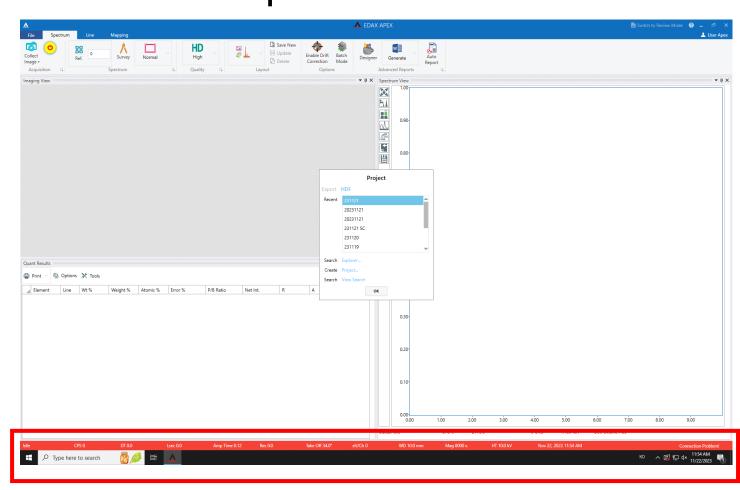

- If the message "connection problem!" appears below the EDS screen
- Turn off the EDS PC and turn off the black EDS detector tick behind the SEM monitor
- Turn on the EDS detector again after 10 seconds and then turn on the EDS PC


## If you encounter a problem while using SEM 3

■ If a problem occurs after of weekdays 09:00~18:00



- Take a picture of the entire monitor screen (or the location where the problem occurred) as above and write down the details of the situation in the logbook.
- 2. Send the above information to the person in charge's email (<u>kale@unist.ac.kr</u>).

- 2. Write a large note on the equipment monitor saying that the equipment is unusable.
- 3. The person in charge will come to work the next day to check the equipment.

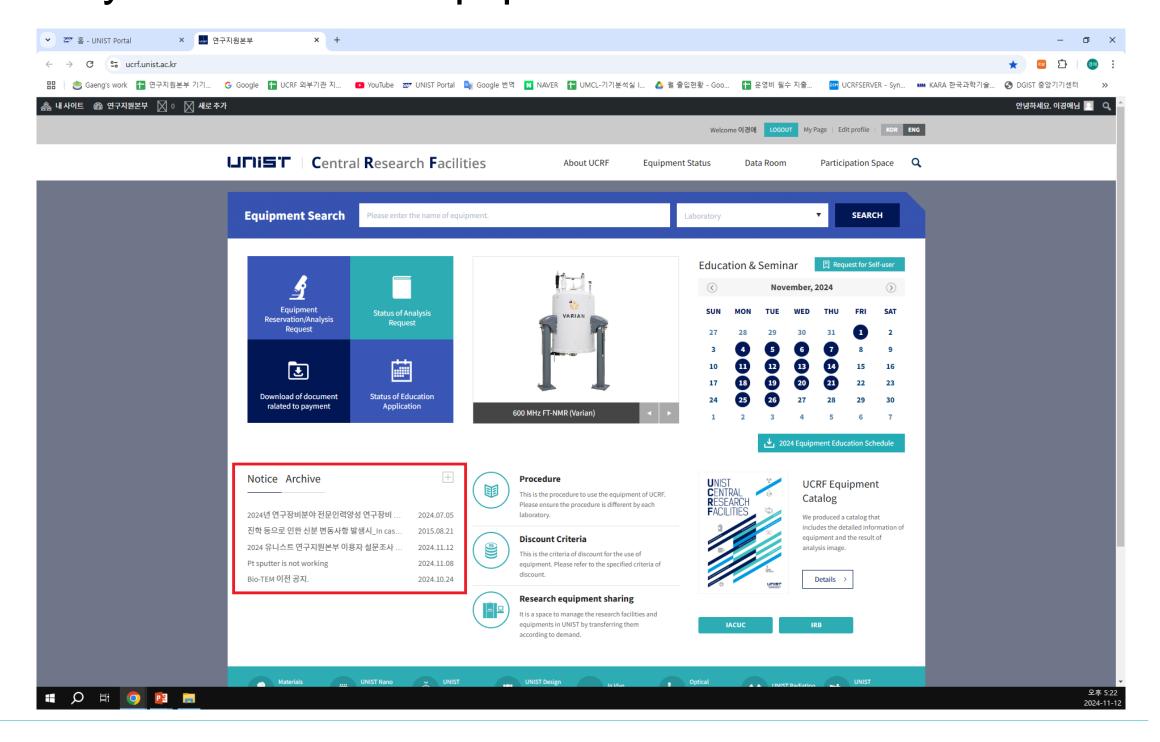




#### **Energy Dispersive X-ray Spectroscopy**





#### www.edax.com

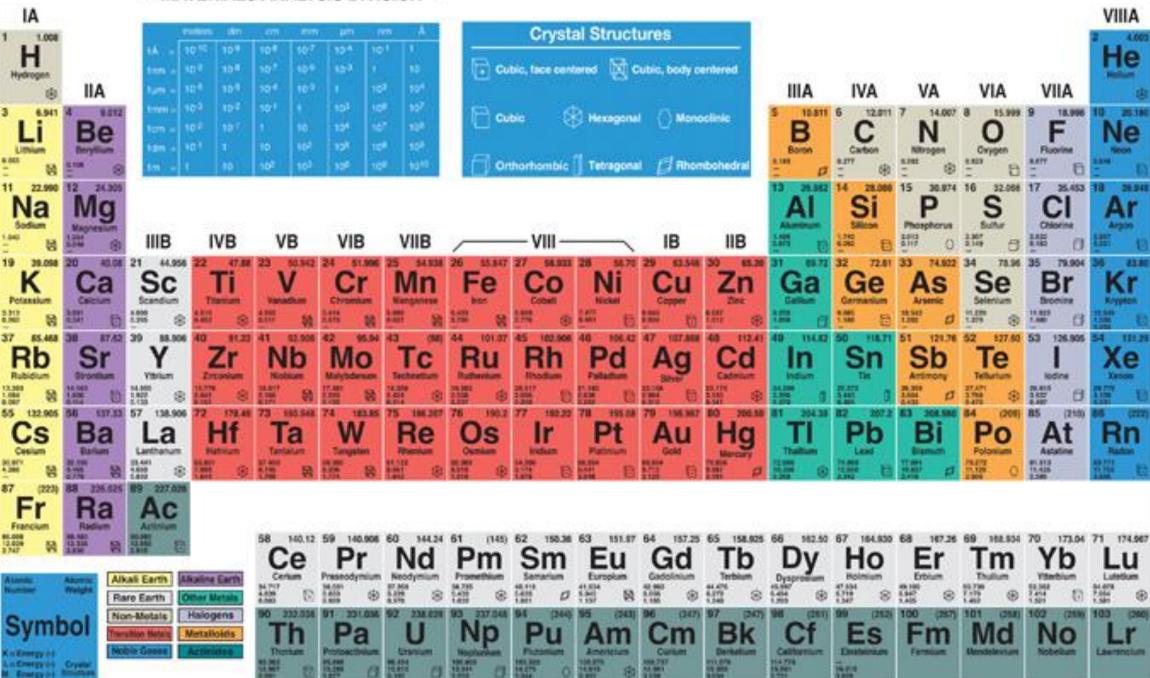

- 1. Click the [Electron Beam]
- 2. Select the acceleration voltage in [Vacc.]★
  (1.5 times kV of the x-ray value of the element
  to be observed or unknown specimens: 20 kV)
- 3. Select beam current (15~25) in [Set le to]
- 4. Click [Close]
- 5. Select [Probe Current] appropriately.
- 6. Move to the position of the specimen to be measured and adjust the magnification.

# **Energy Dispersive X-ray Spectroscopy**

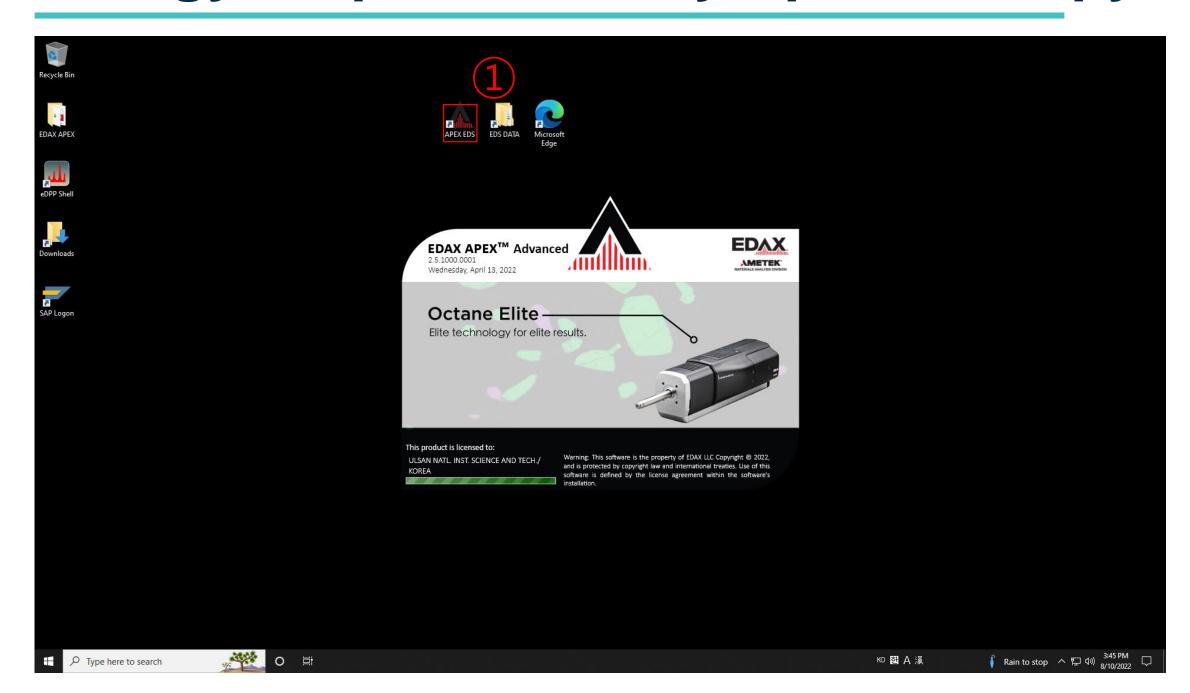


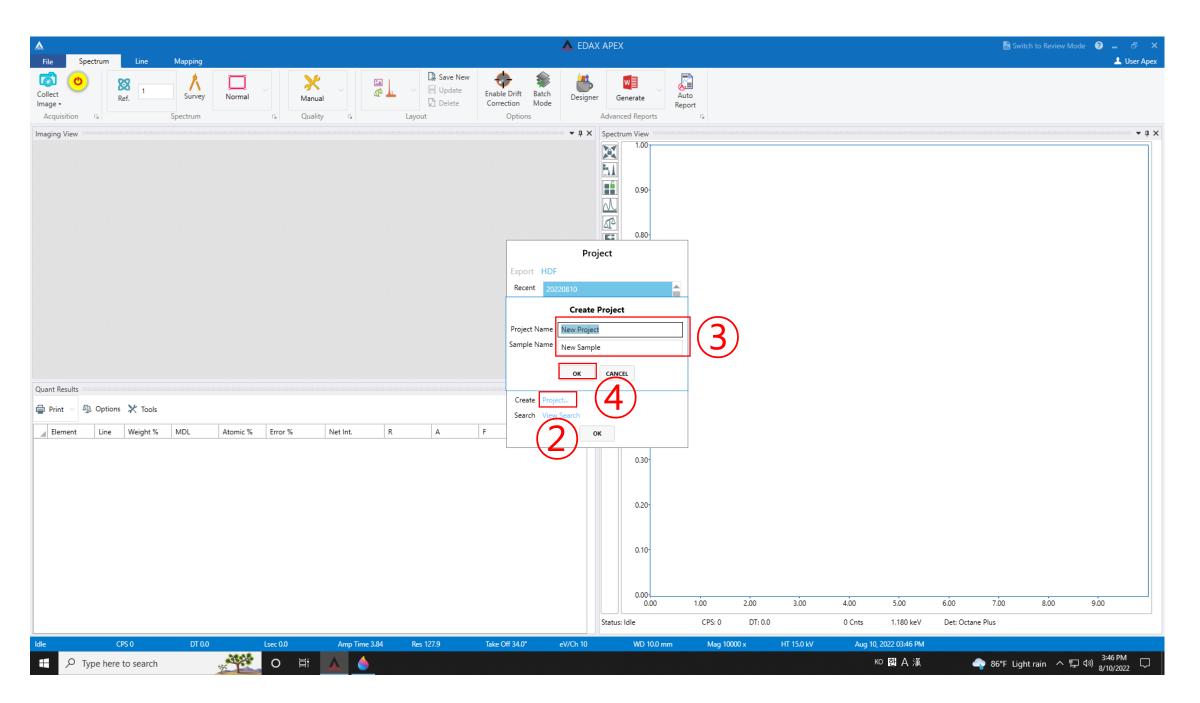


- 1. Click [APEX]
- 2. Click [Create Project...]
- 3. Enter [Project Name] and [Sample Name]
- 4. Click [OK]




## **Energy Dispersive X-ray Spectroscopy**

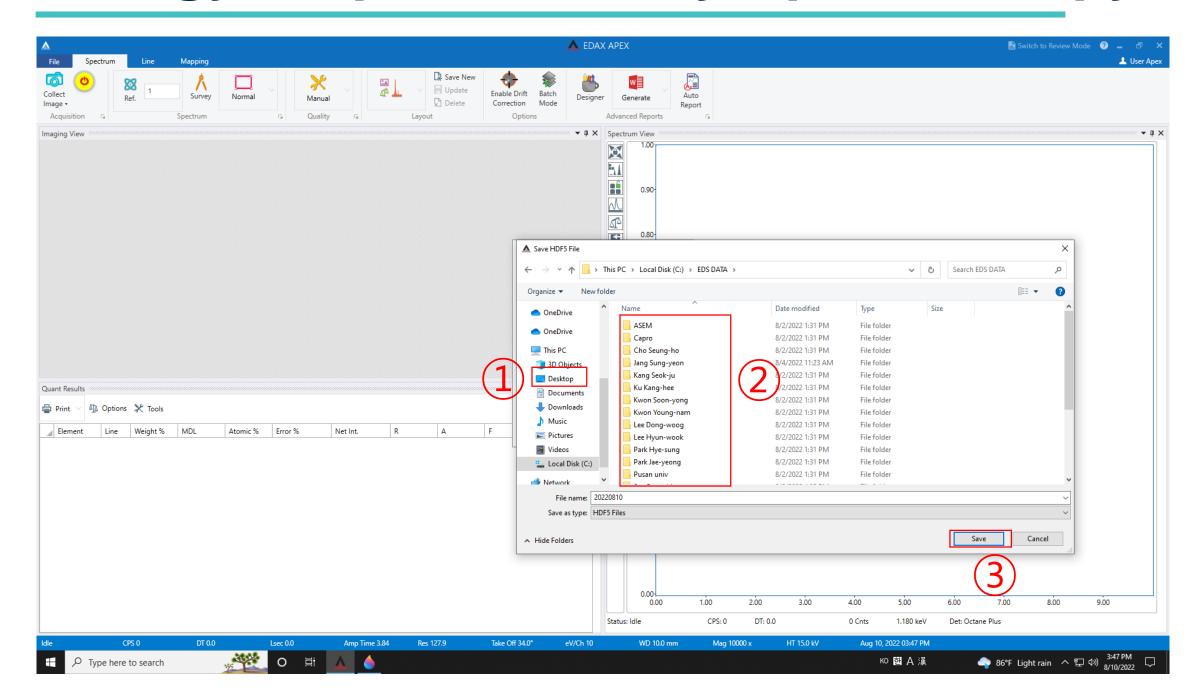

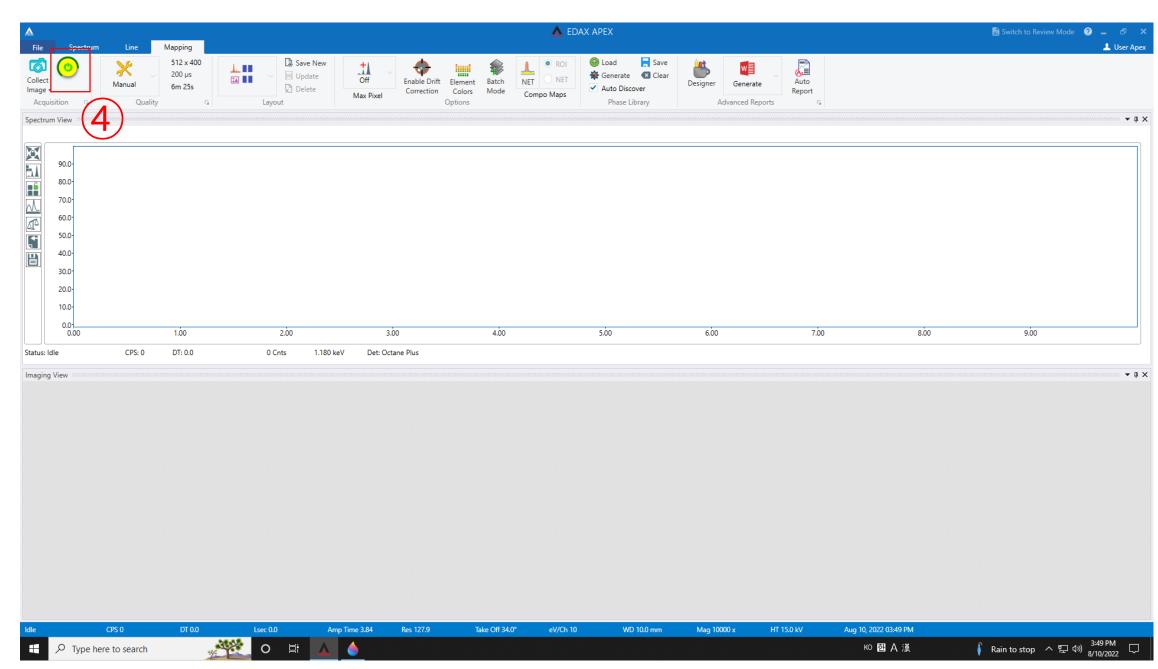


- 1. Click [Desktop] and click [EDS DATA]
- 2. Create a folder for each professor's lab, and create your own folder.
- 3. Click [Save]
- 4. Click [Detector]




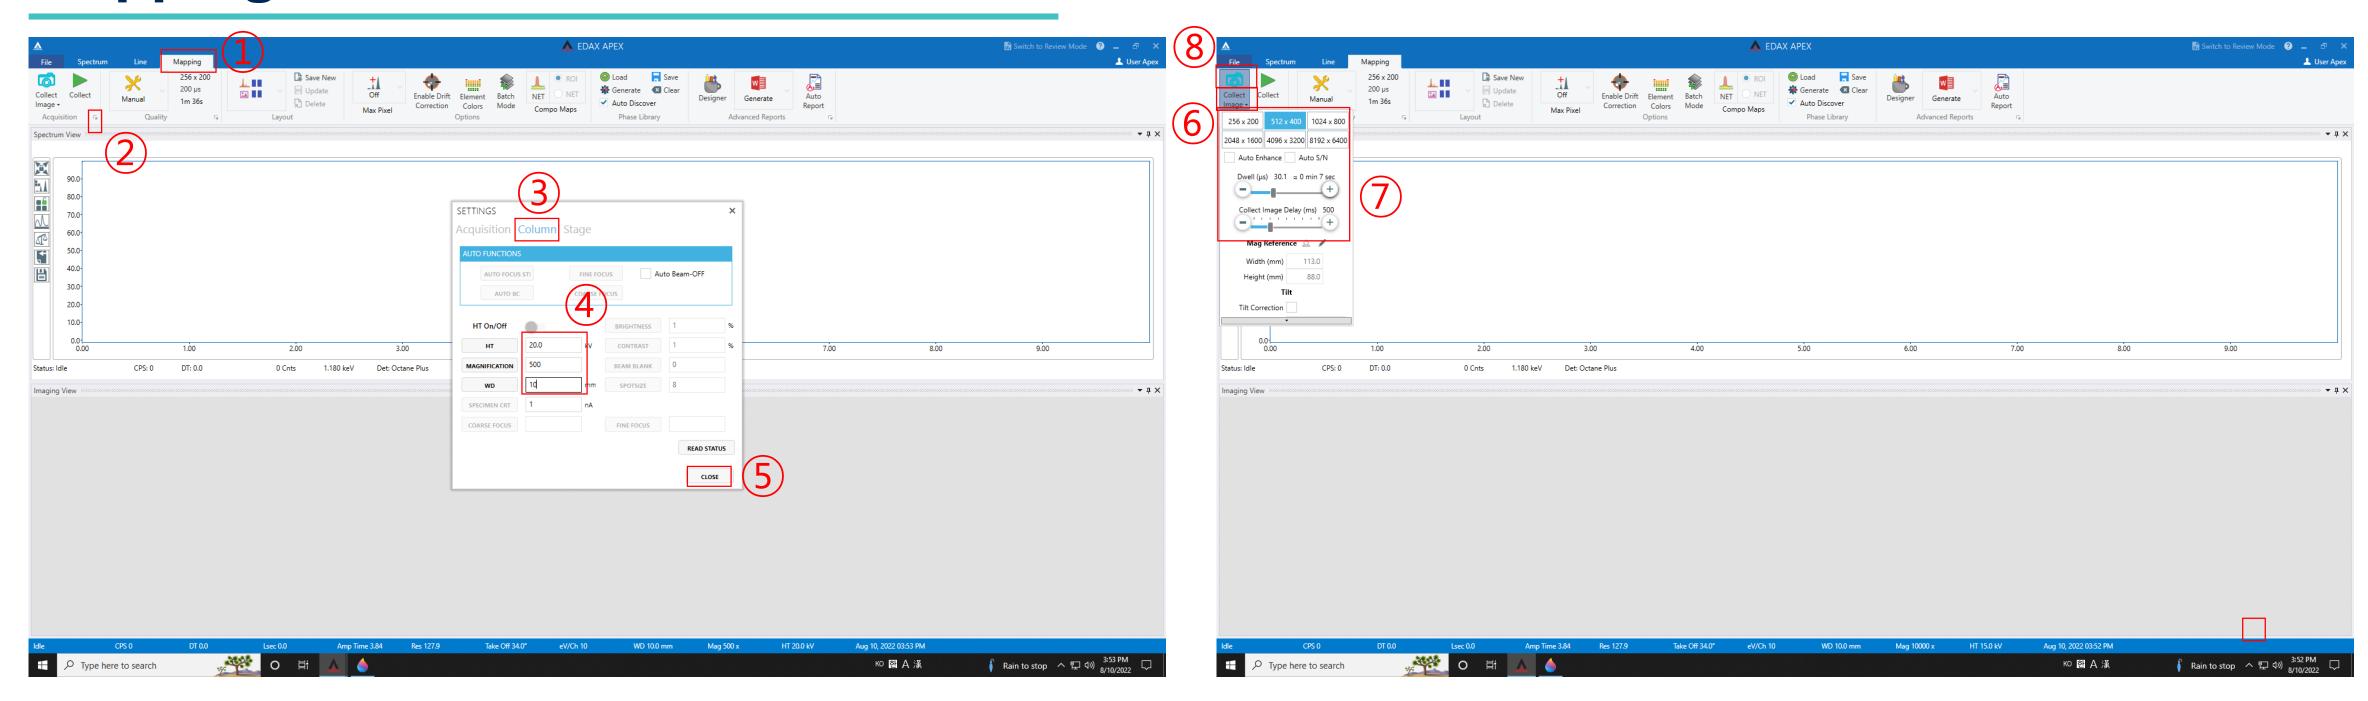

- 1. Click [Mapping] and click the arrow next to [Acquisition], click [Column]
- 2. Enter [HT] and [MAGNIFICATION], [WD]=6, click [CLOSE]
- 3. Click [Collect Image]
- 4. Click [Camera]




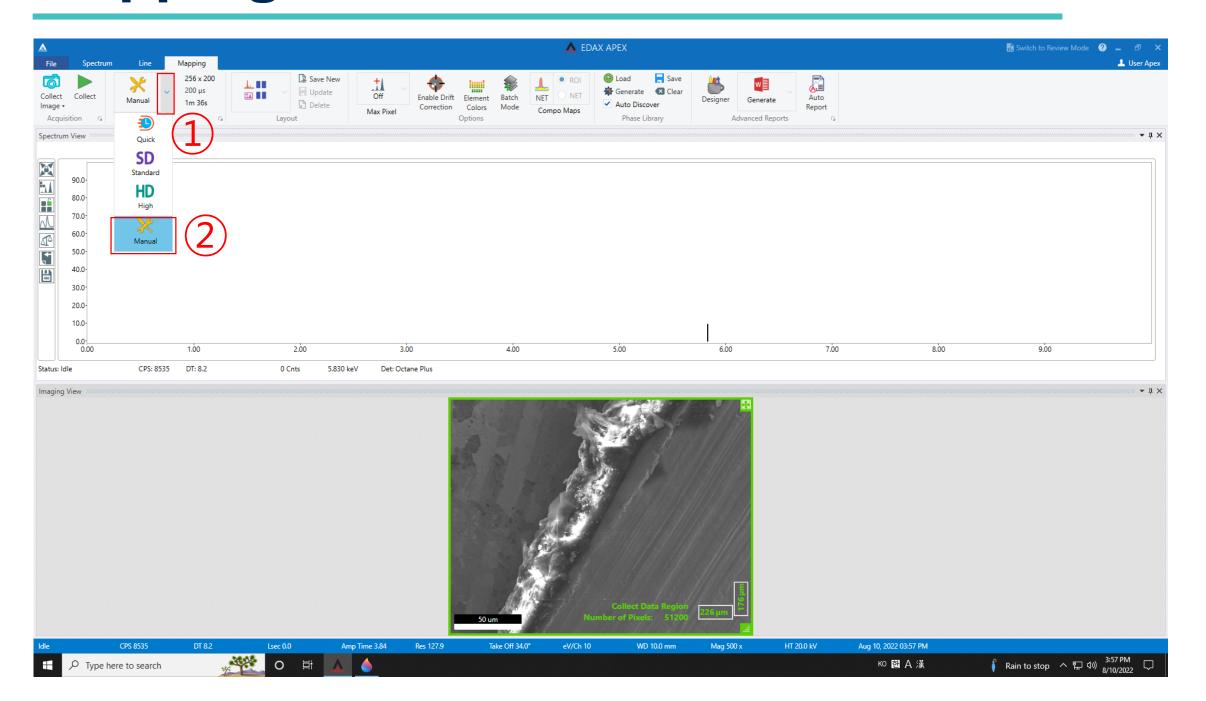


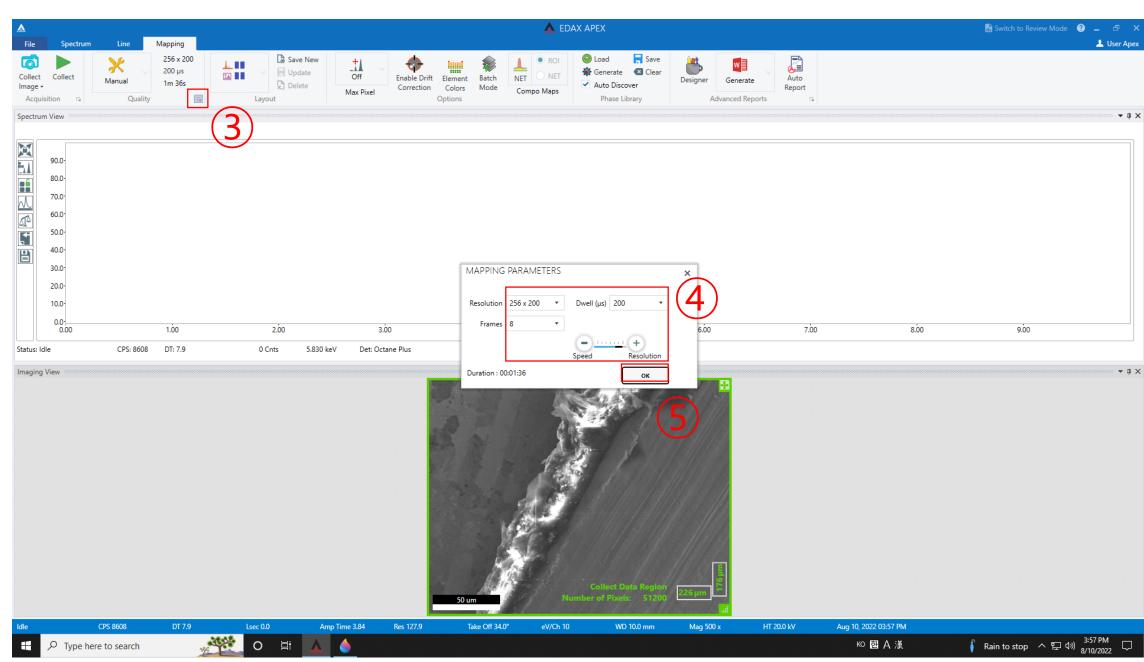

- 1. Click the arrow next to [Manual] and Click [Manual]
- 2. Click the arrow next to [Quality]
- 3. Adjust [Resolution] and [Dwell], Frames appropriately
- 3. Click [OK]




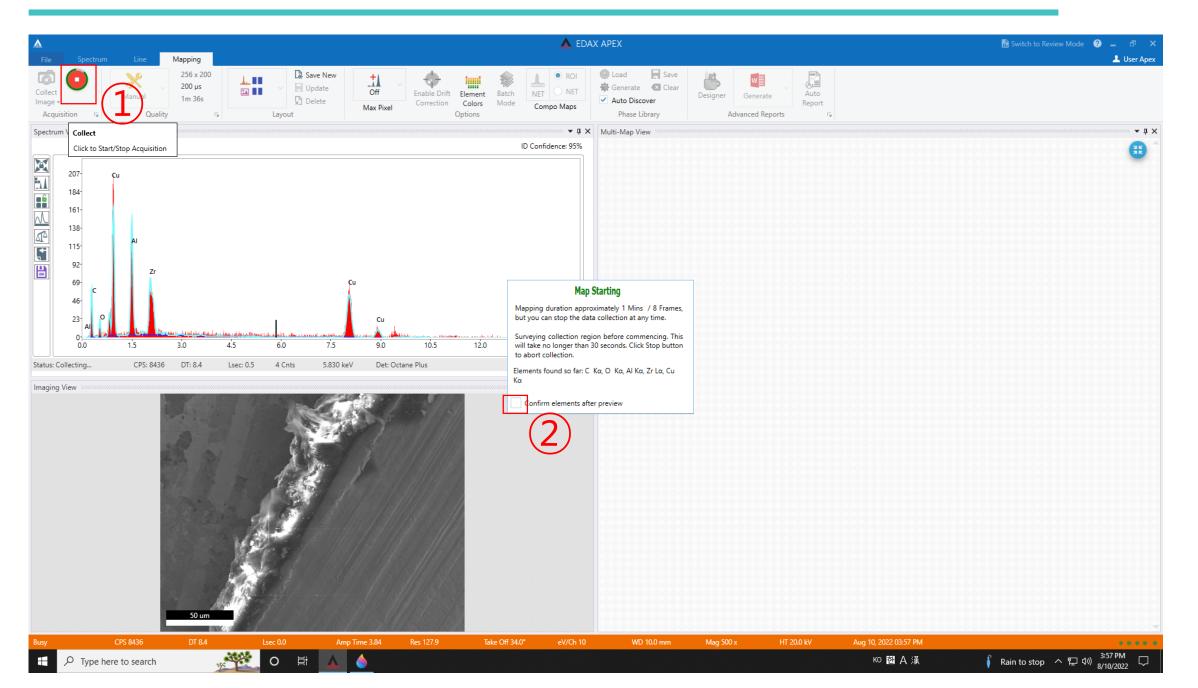


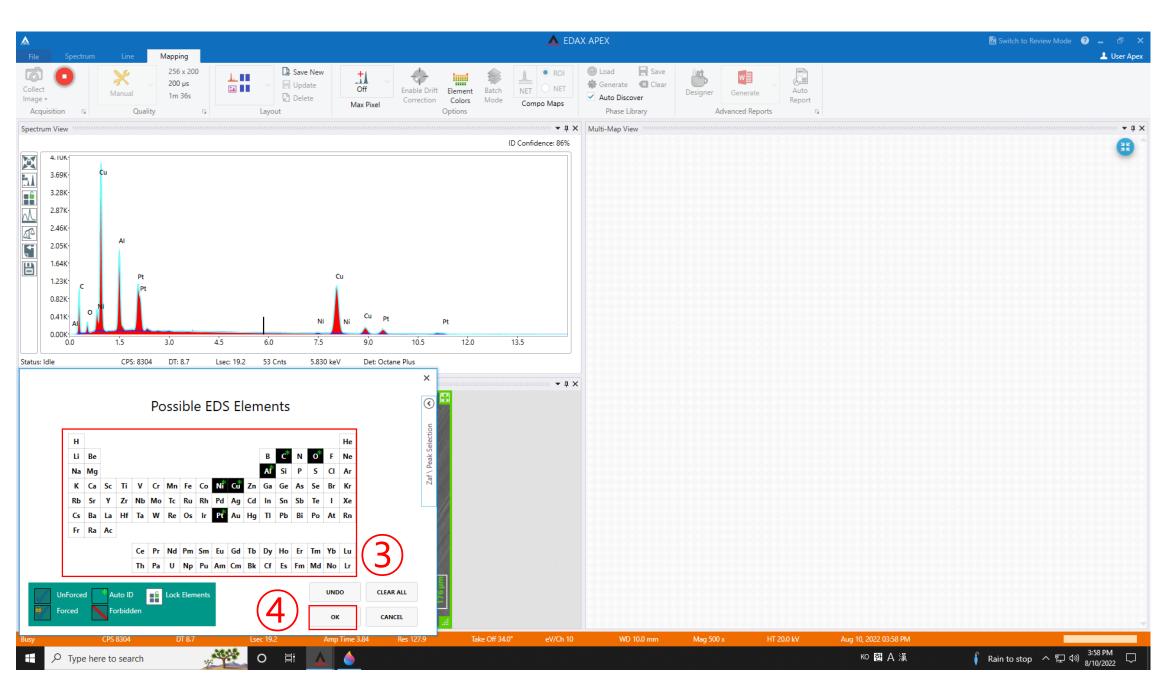

- 1. Click [Collect]
- 2. Check [Confirm elements after preview]
- 3. Just click on the element of interest to make it black and click [OK]
- 4. Click [OK]




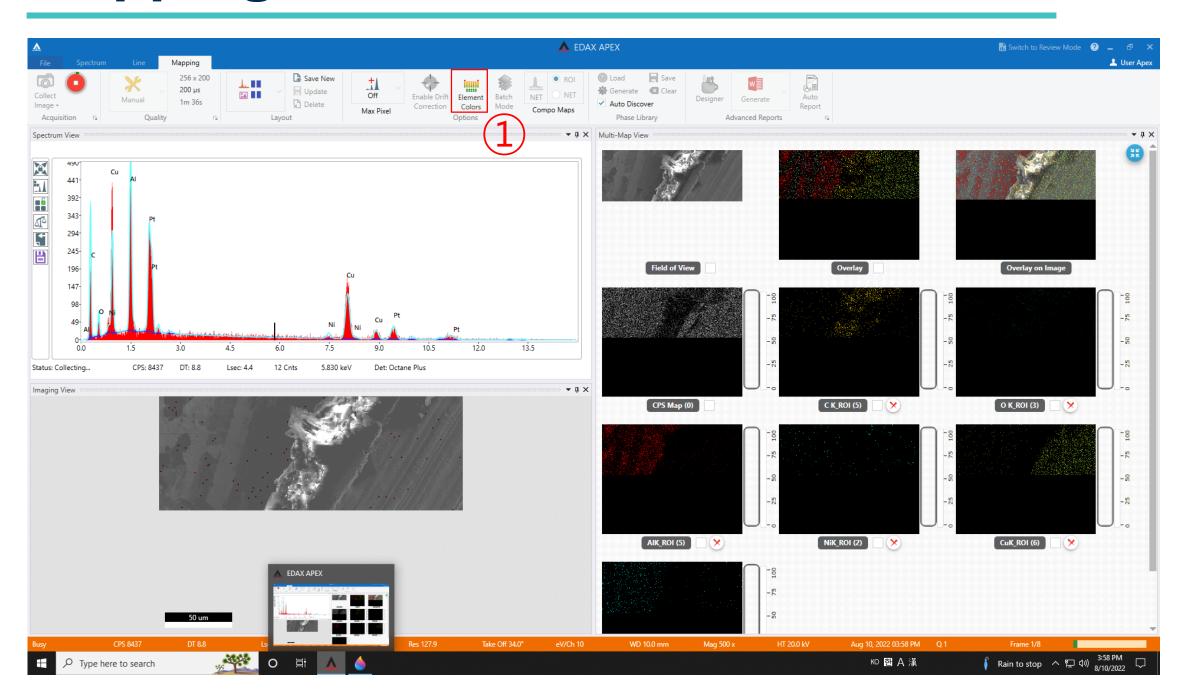


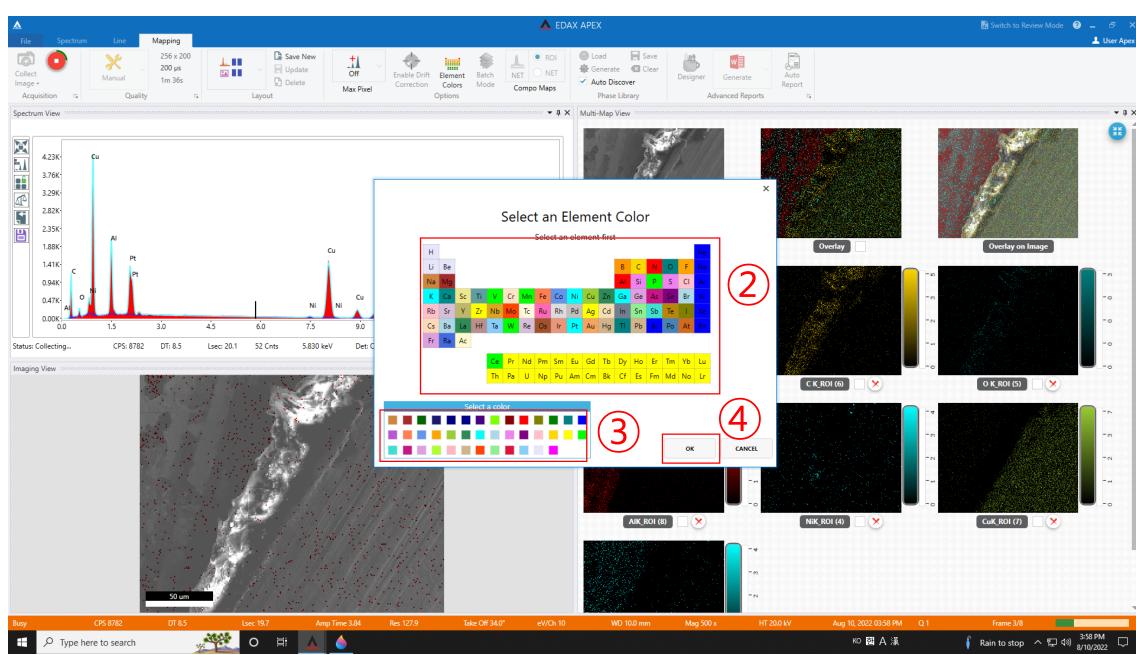


- 1. Click [Element colors] to change the color of an element
- 2. Select the element you want to change
- 3. Choose the color you want to change
- 4. Click [OK]




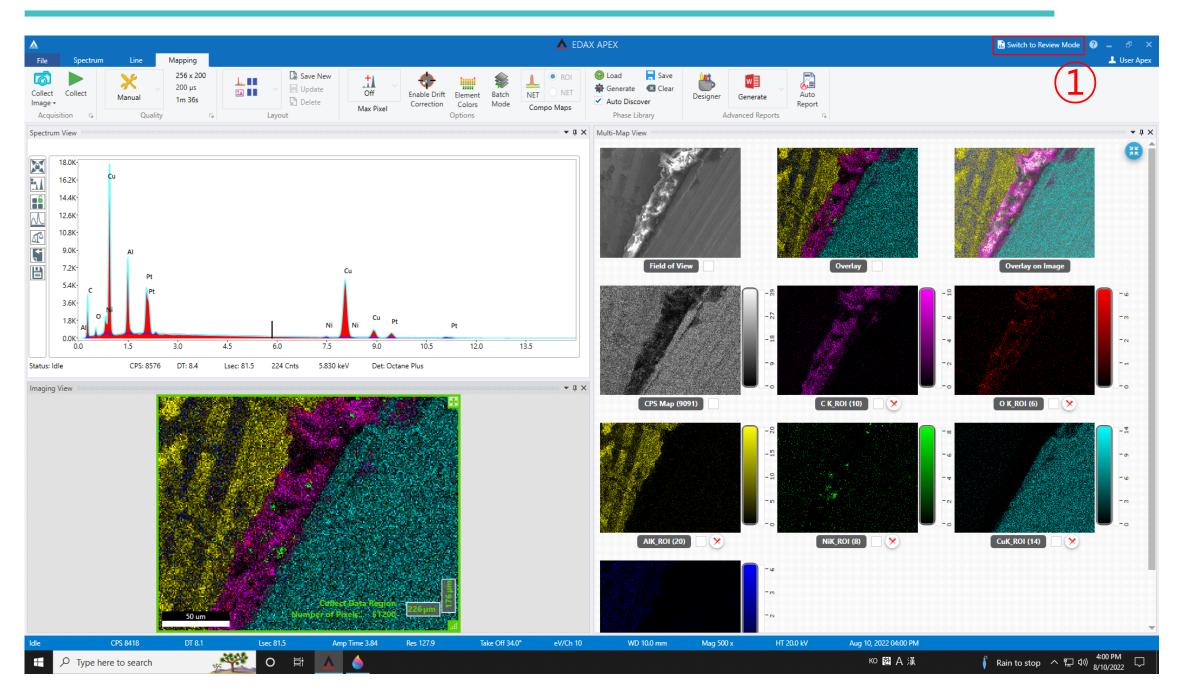

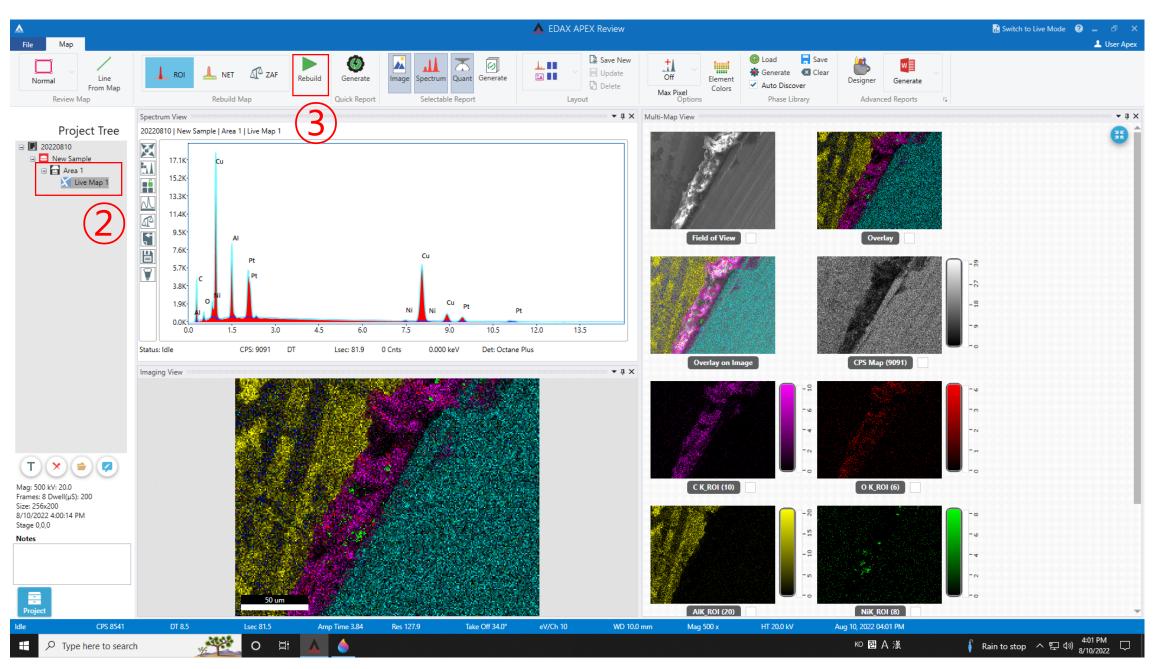



- 1. Click [Switch to Review Mode]
- 2. Double click on data in Project Tree
- 3. If you want to change the mapping element, click [Rebuild]

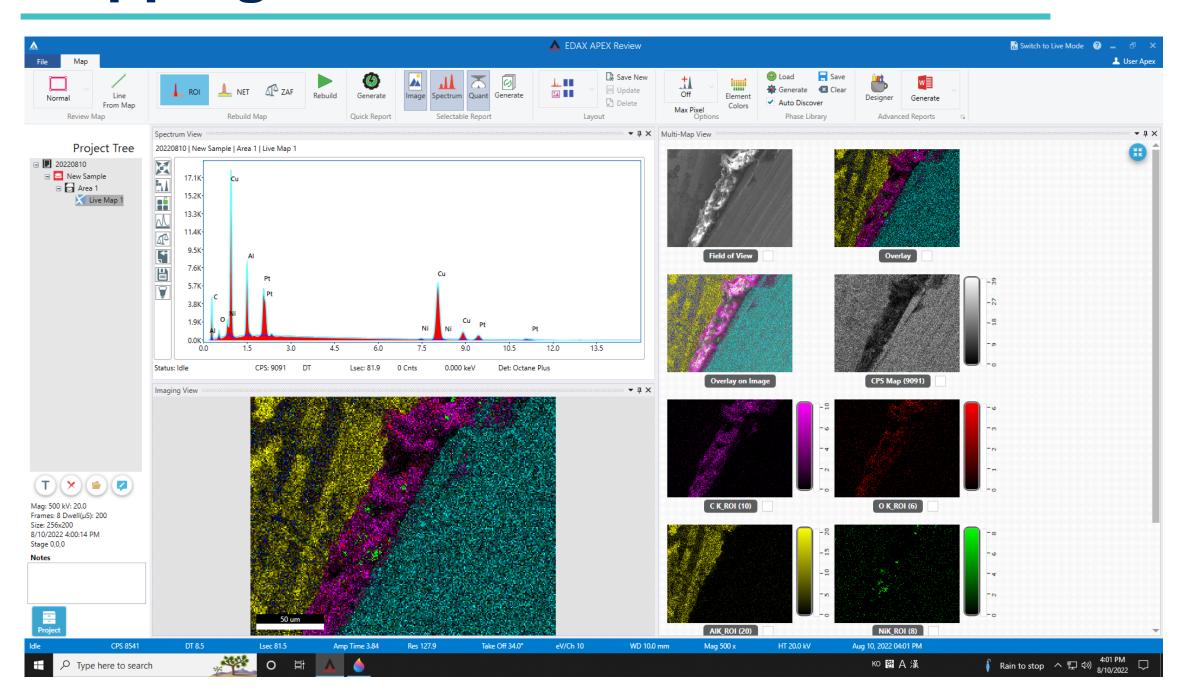

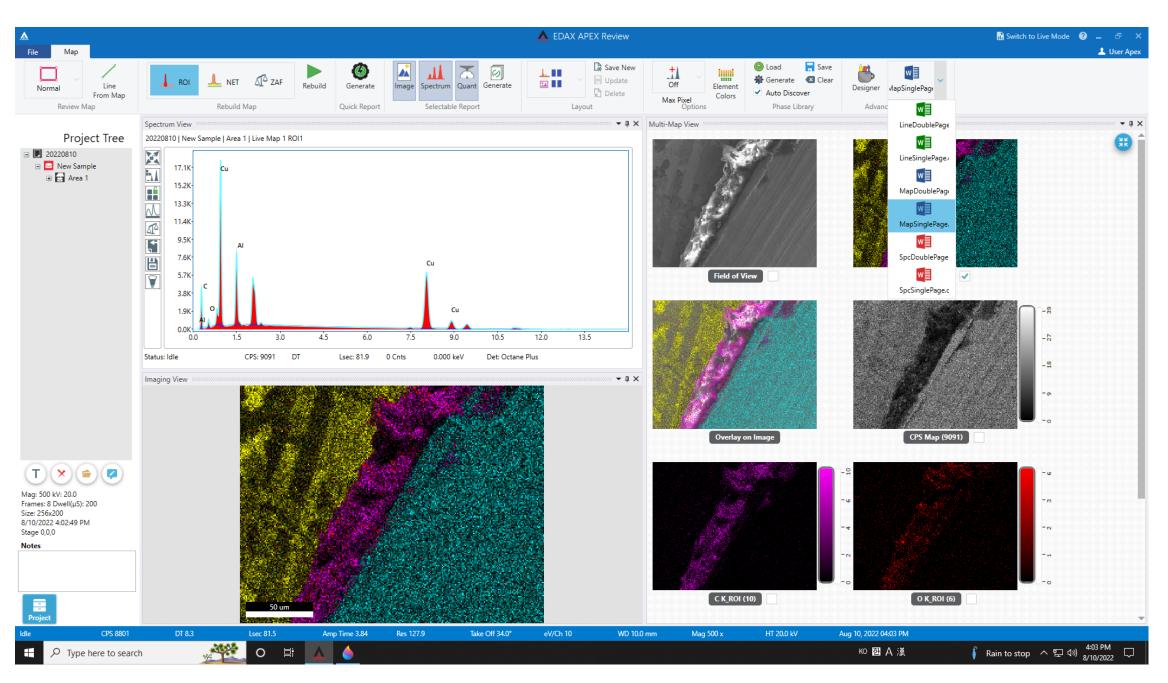


- 1. Select the element you want and make it black
- 2. Click [OK]
- 3. Wait for the conversion to complete
- 4. Choose the template you want

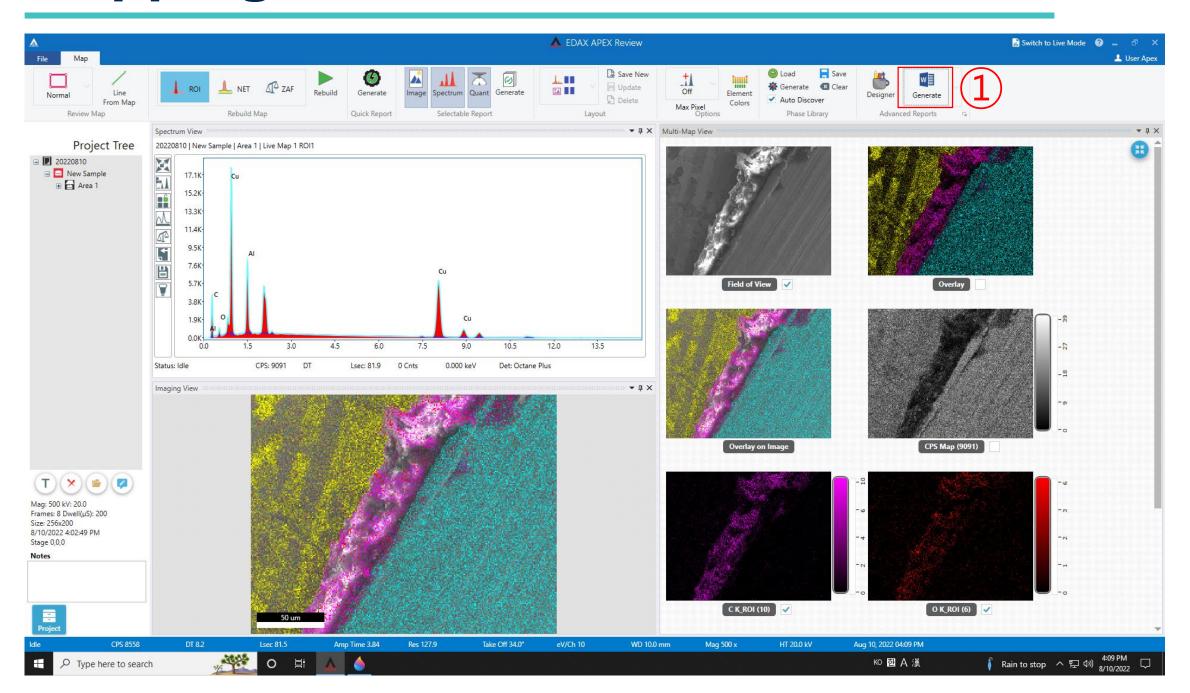


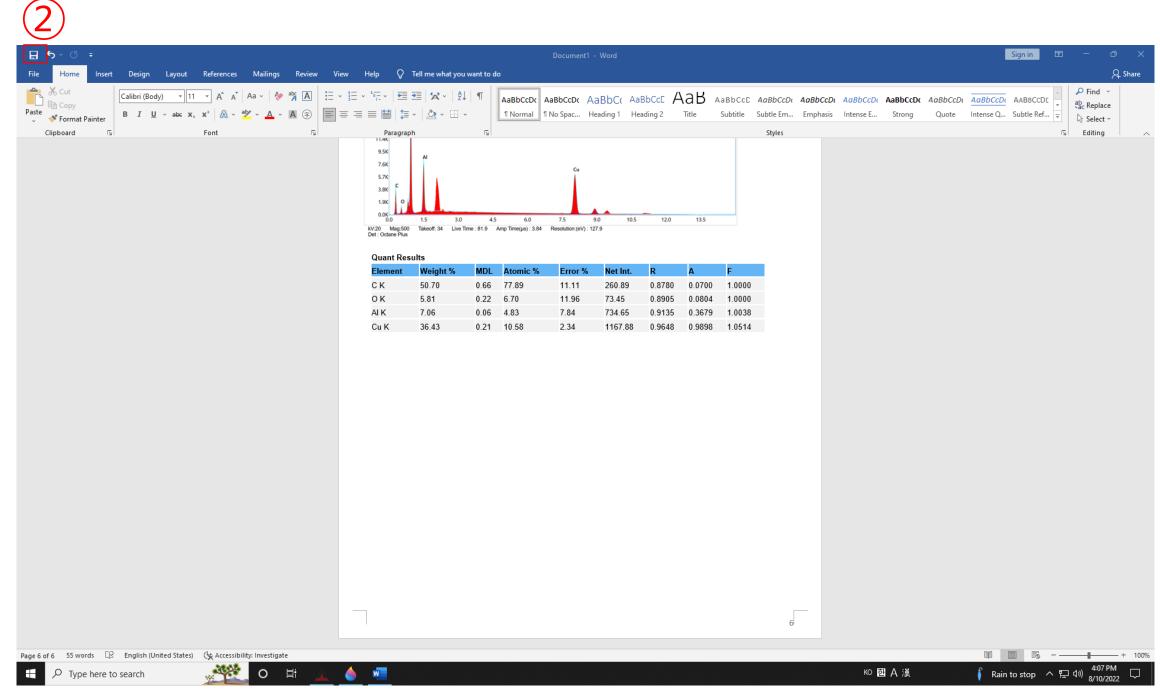

- 1. Click [Generate]
- 2. Create a folder for each professor's lab, and create your own folder.
- 3. Click [Save]




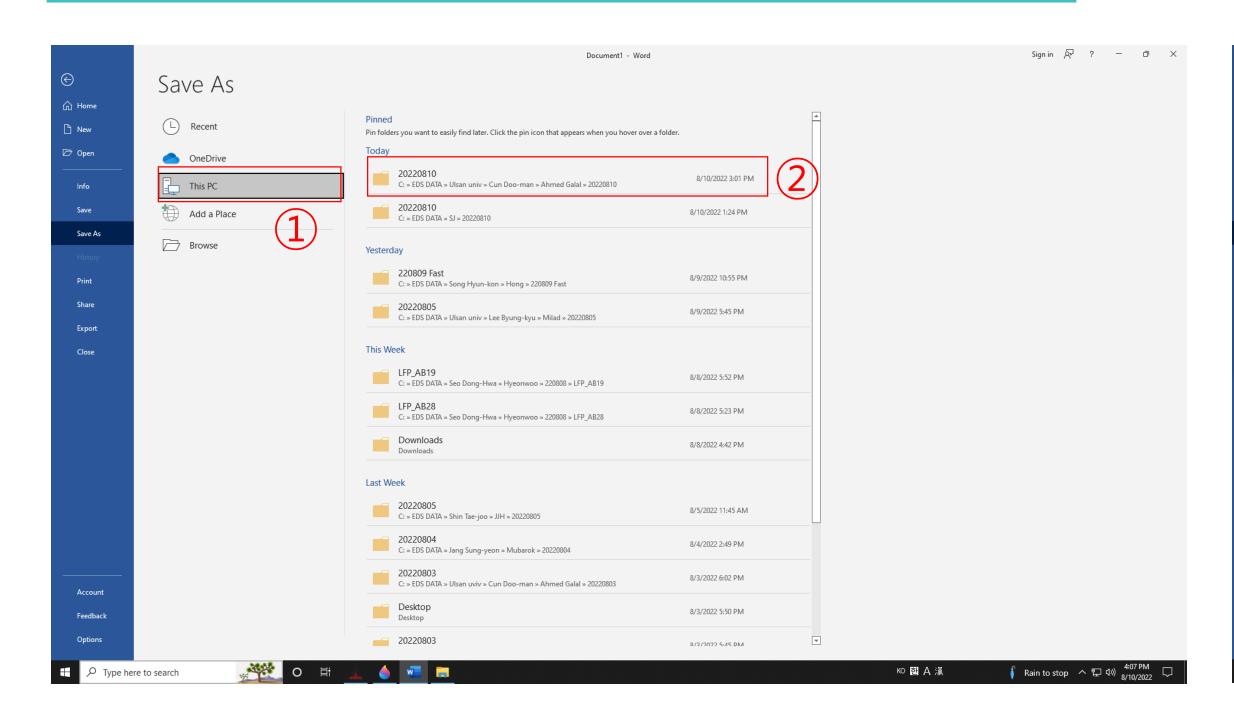


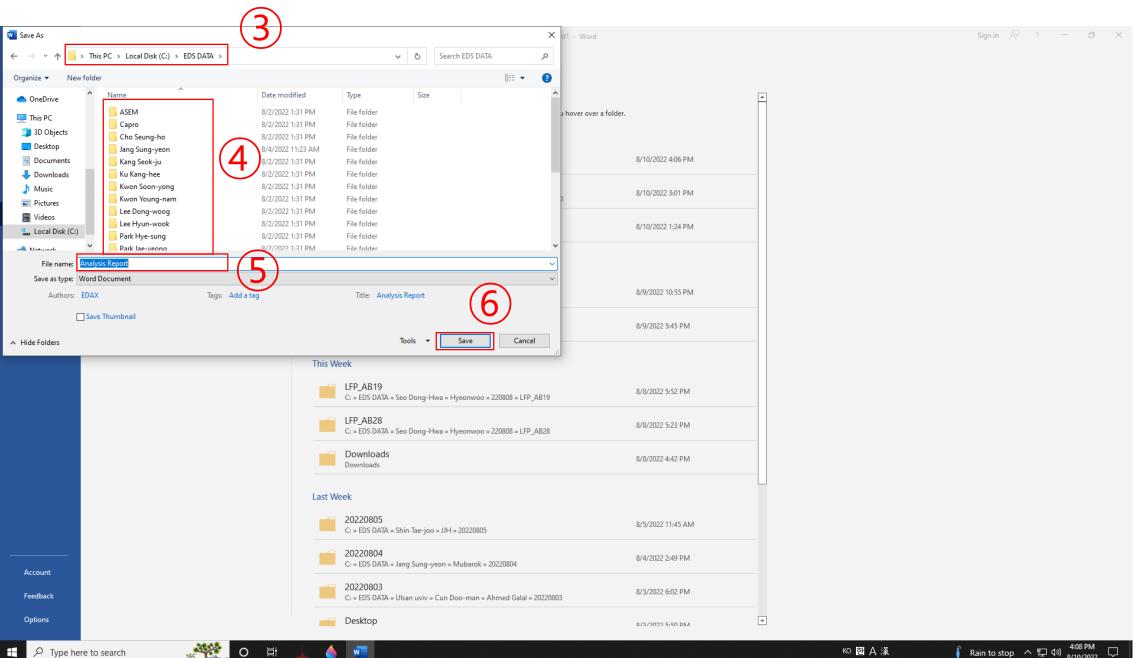

- 1. Click [This PC]
- 2. Find the folder you created at startup
- 3. Enter the file name
- 4. Click [Save]



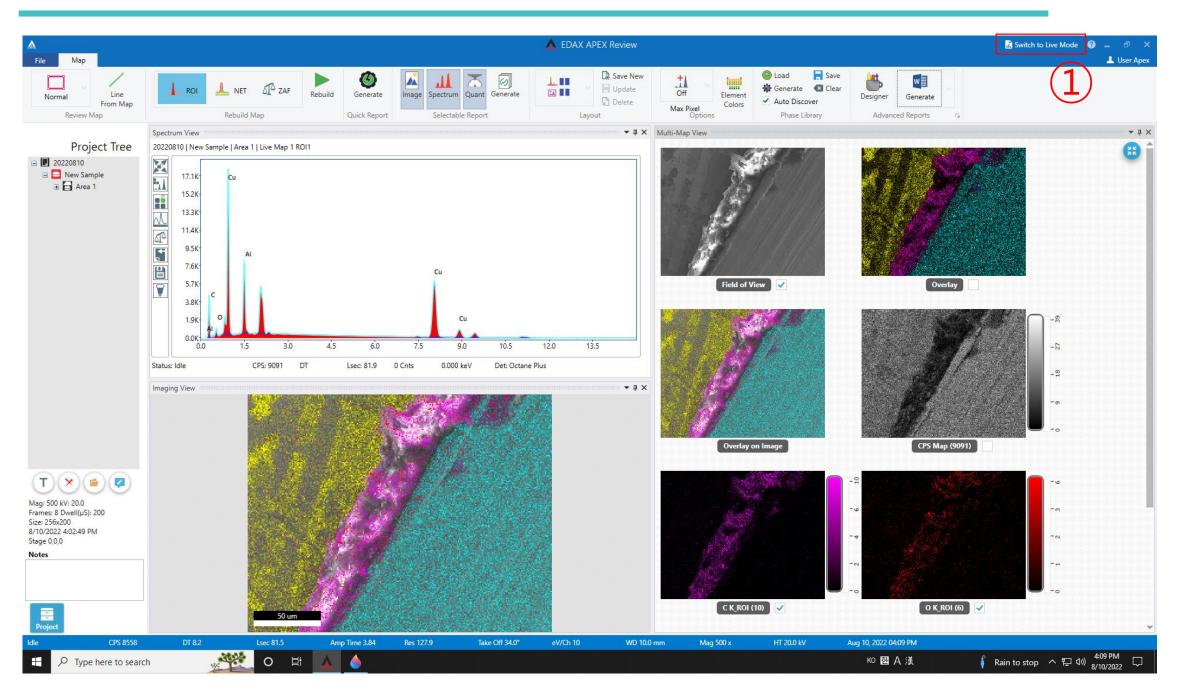

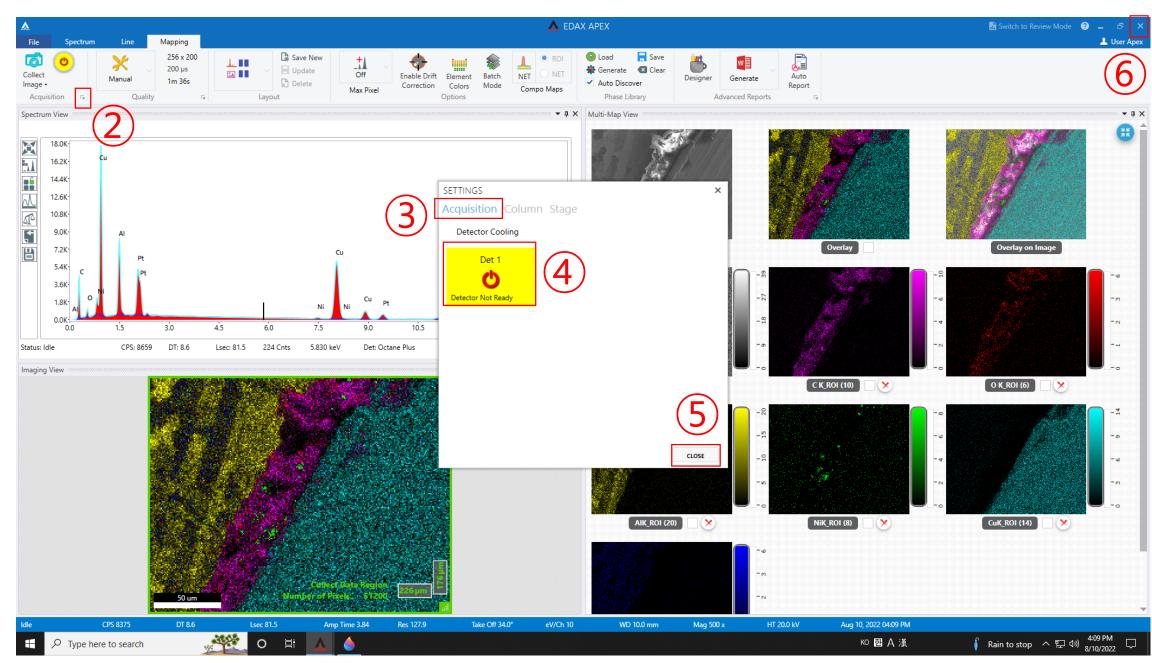


- 1. Click [Switch to Live Mode]
- 2. Click the arrow next to [Acquisition]
- 3. Click [Acquisition] and click [detector]★
- 4. Click [CLOSE] and click [X]




### **Create Account**

#### www.ucrf.unist.ac.kr

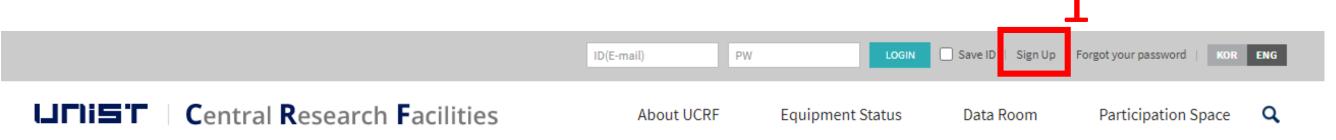



- 1. Click [Sign up]
- 2. Click [UNIST Member]
- 3. Input [Portal ID/PW] → Click [Confirm]Please check your information
- 4. Input professor name in [Principal Investigation]
  - → [Professor search] → professor name
- 5. Click [Create Account]

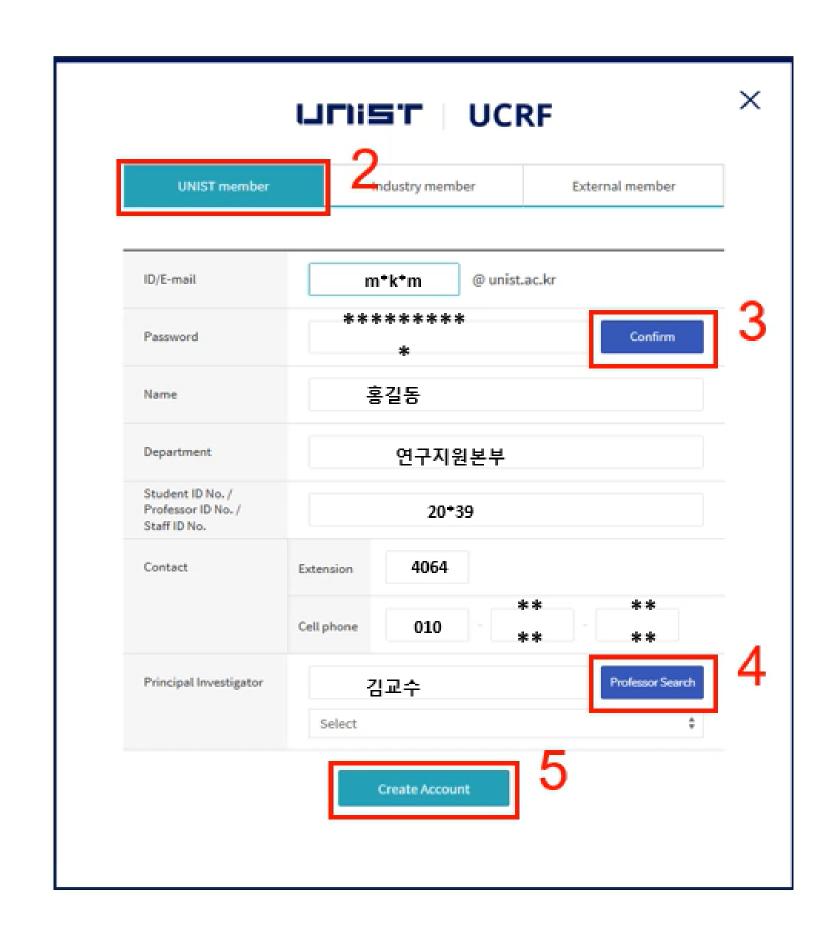

### **Access Permissions Application**

#### www.ucrf.unist.ac.kr

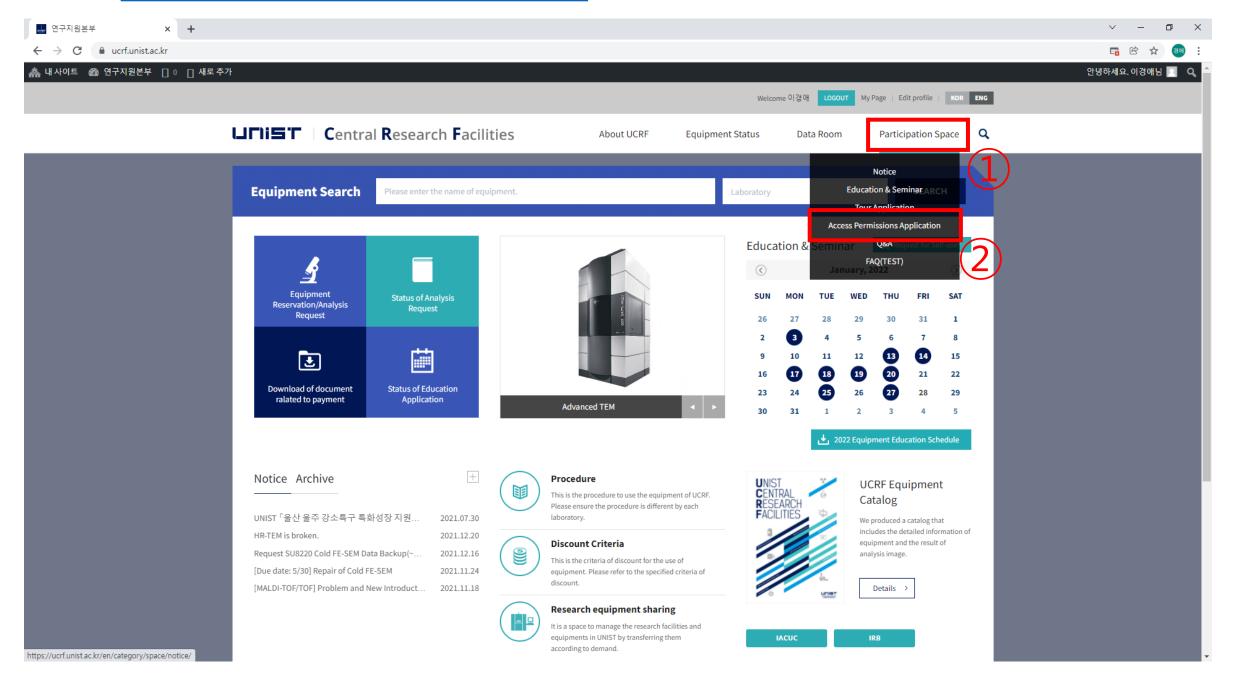


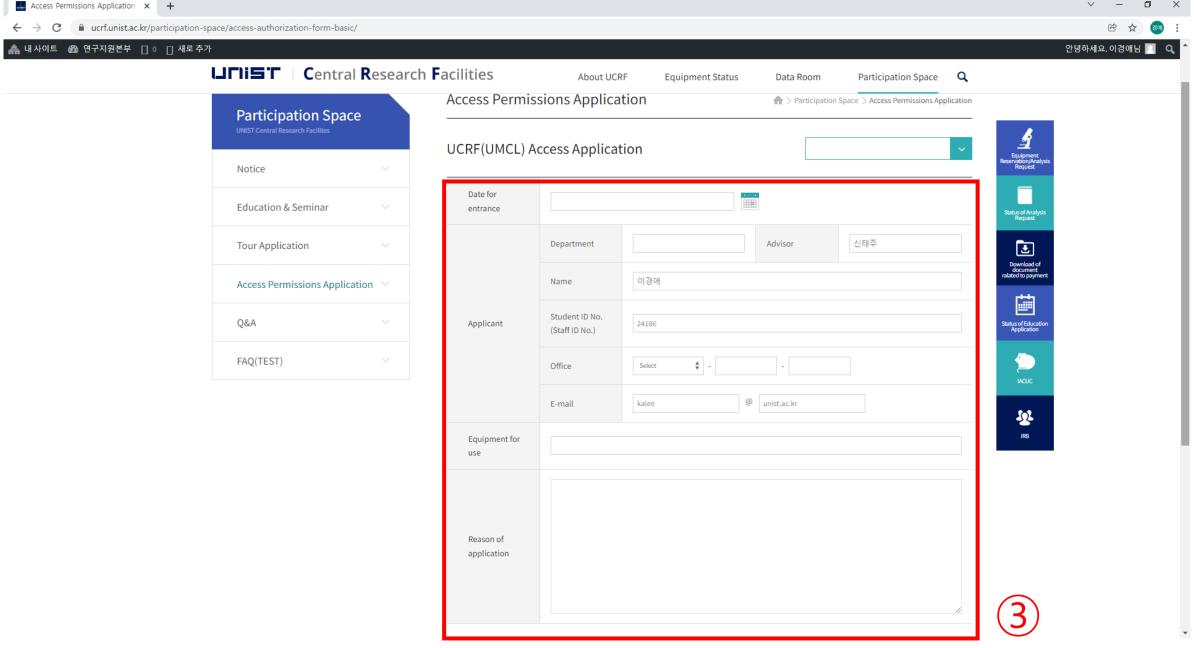

- 1. Click [Participation Space]
- 2. Click [Access permissions Application]
- 3. Fill out the UCRF(UMCL) Access Application form
- 4. Click [Apply]

- When reissuing the ID card, you must apply for access again on UCRF website.
- Access Authorization Officer:
   Kang Yeong-bi(052-217-4168)

### Request for Self-user

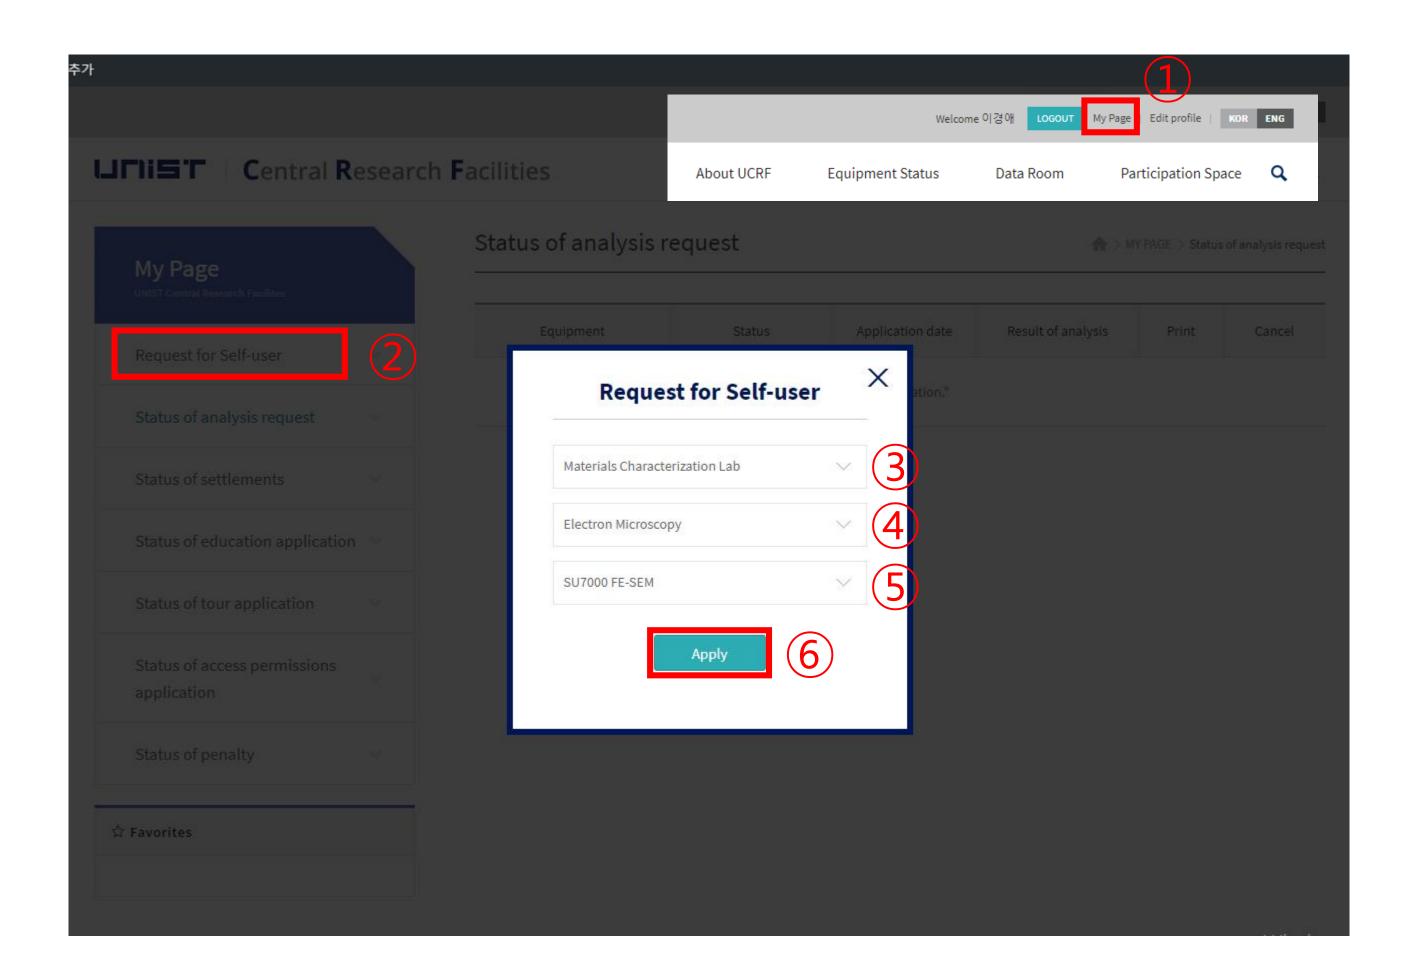


### After pass the test,

- Login UCRF website
   (www.ucrf.unist.ac.kr)
- 2. Click [My Page]
- 3. Click [Request for Self-user].
- 4. Select [Materials Characterization Lab]
- 5. Select [Electron Microscopy]
- 6. Select [SU7000 FE-SEM]
- 7. Click [Apply]


### Reservation

### portal.unist.ac.kr - Research Equipment - Equipment reservation/input result

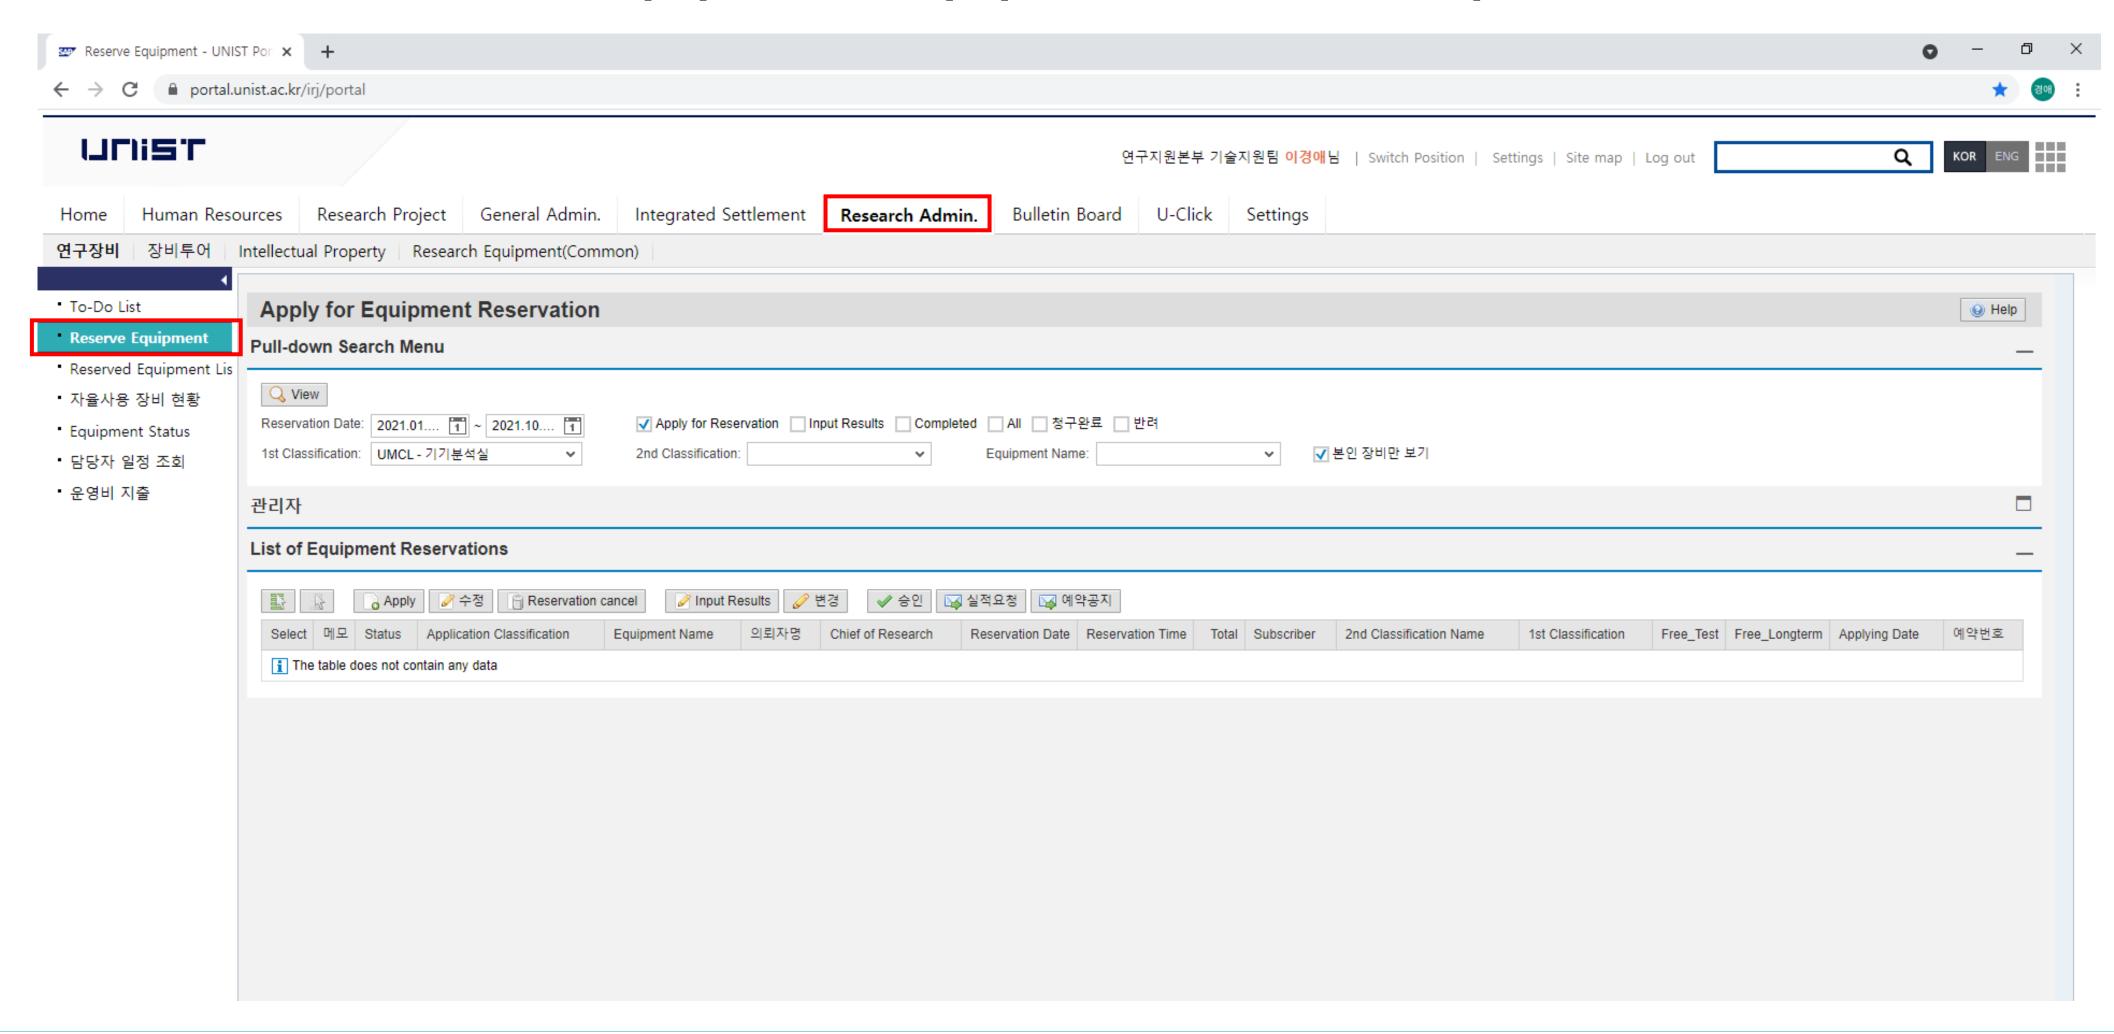

### Reservation


### portal.unist.ac.kr - Research Equipment - Equipment reservation/input result

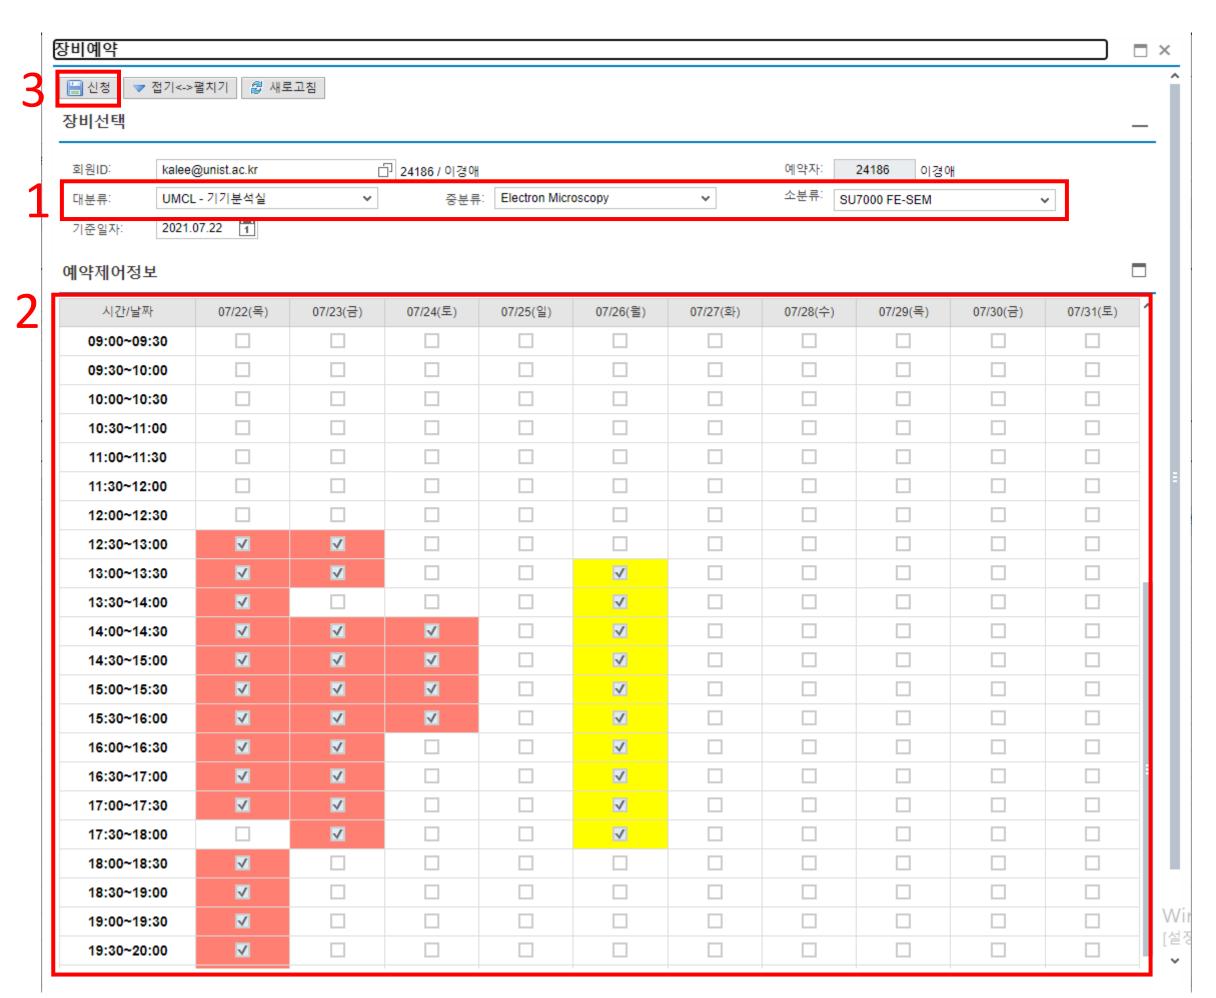

- 1. Select the classification and equipment
- 2. Select the time you want on white box
  - Yellow box : my reservation
  - Red box: others reservation
- 3. Click [Application]

#### **Reservation cancel**


### portal.unist.ac.kr - Research Equipment - Equipment reservation/input result

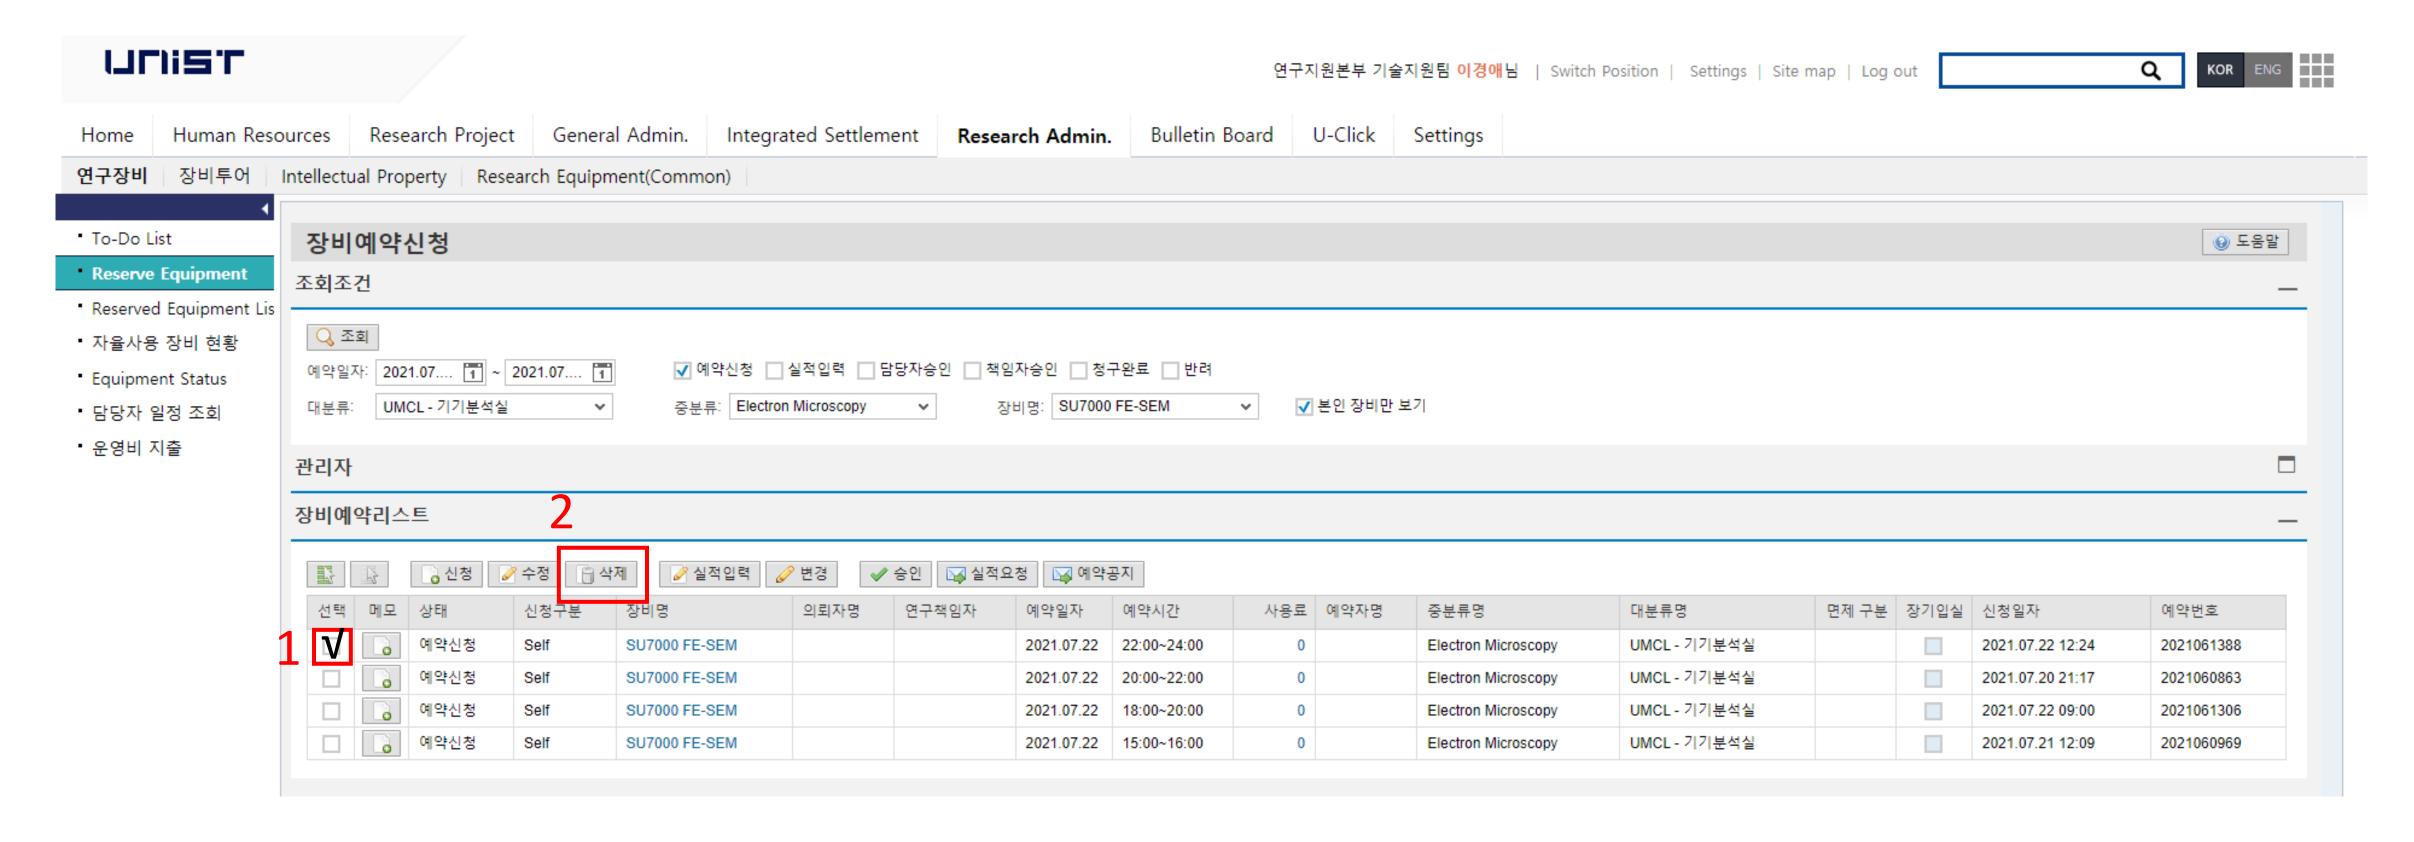



### Input result

### After measurement, you have to input result instead of filling in log sheet

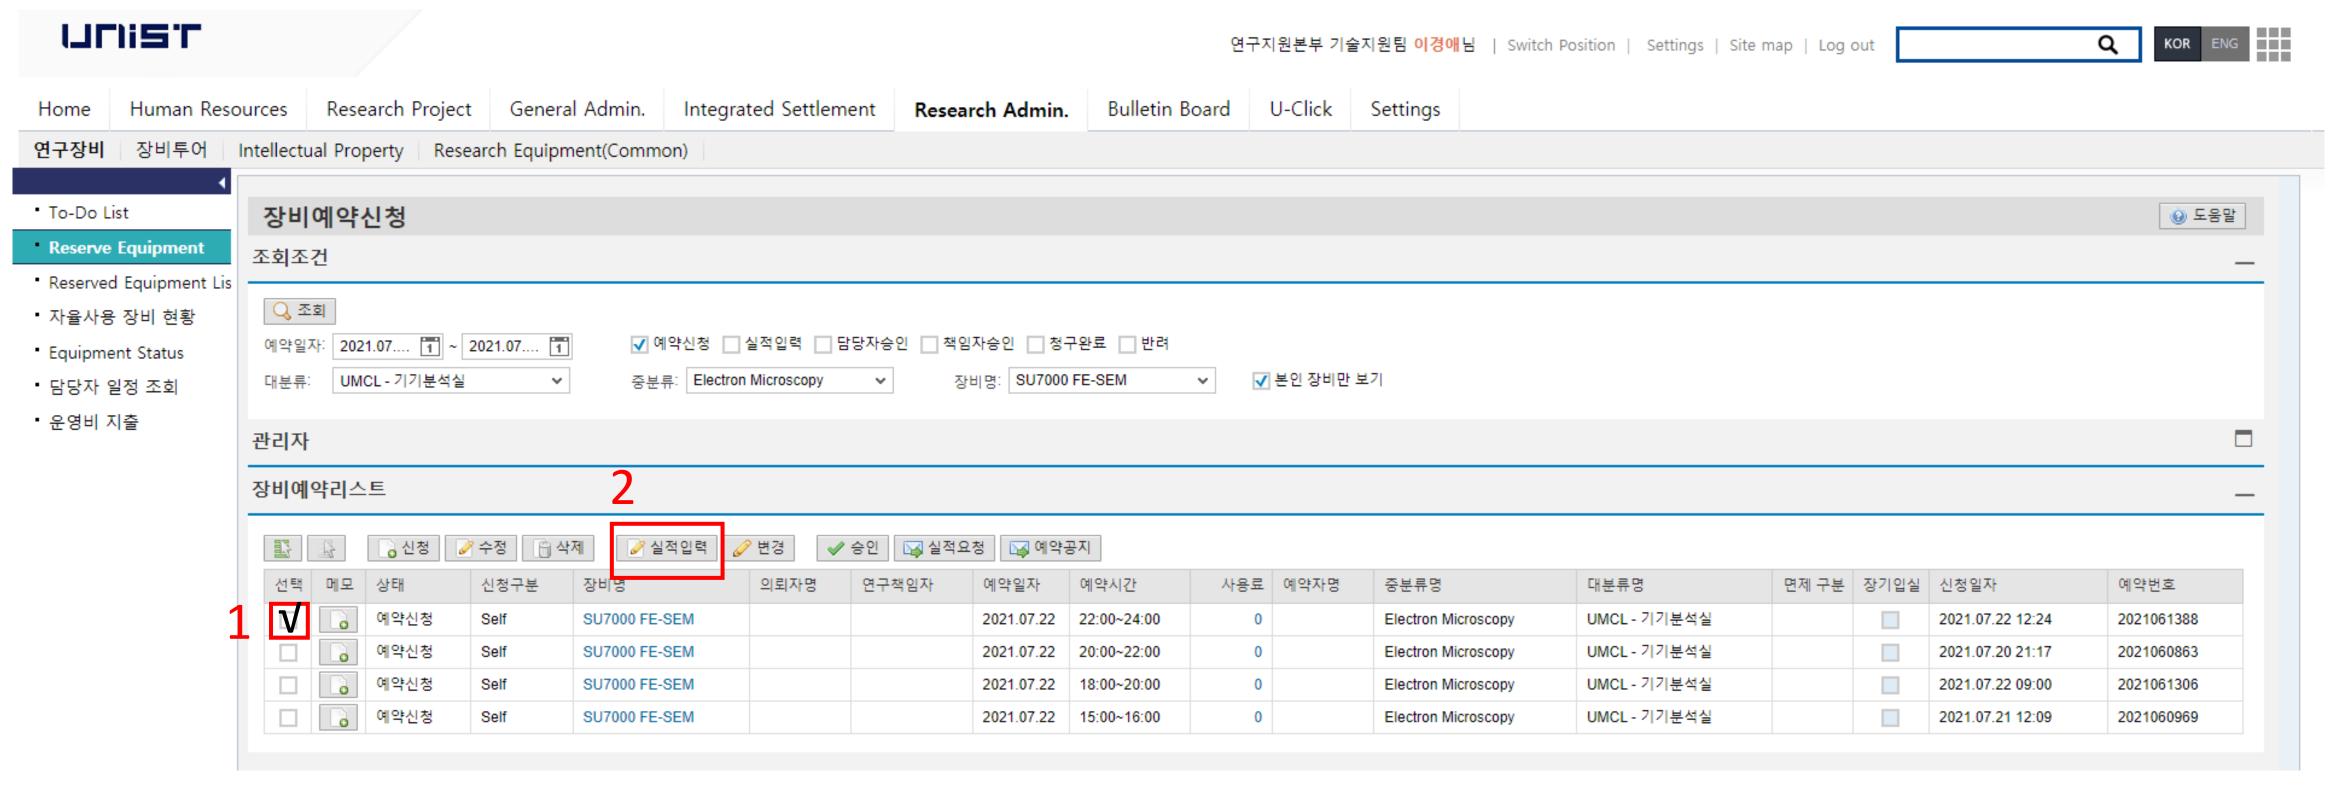

- 1. Select the reservation
- 2. Click the [Input result]
- 3. Check the information and click [Save]



#### **Article 1. Access**

- ① A person who wishes to be authorized access to UMCL must obtain approval from the manager in charge after submitting an application form to "Access Permissions Application" of the "Participation Space" menu on the UCRF homepage (http://ucrf.unist.ac.kr).
- ② A person who wishes to enter UMCL without access authority shall be accompanied by the equipment manager or shall obtain approval for access from the equipment manager.
- 3 Each user must enter (exit) individually using the pass card with their own identity, and it is prohibited to enter using another person's pass or to enter together without permission.
- ④ A person who uses UMCL at night (PM18-AM09 on the next day) or on holiday must enter after establishing personal safety and protection rules (accompanying 2 or more people, preparing for an emergency contact, etc.) for lab accidents.
- ⑤ A person who violates above paragraph  $1 \sim 4$  regarding access to UMCL shall be obligated to compensate for all safety and property damage caused by the violation.

#### Article 2. Use of laboratory space

1 A UMCL user must understand and follow the common safety rules for the laboratory (Attachment 1).

- ② A UMCL user on weekends or holidays must fill out the laboratory daily checklist (Attachment 2) provided in each laboratory room, and must submit it to equipment manager, with the signature of the professor(or supervisor) within 3 days from the date of use.
- ③ A UMCL user should clean up the area after using the equipment, and must promptly notify the equipment manager if there is any problem with the equipment or environment. Violation of the notification obligation may result in restrictions on the use of the equipment.

#### **Article 3. Use of Equipment**

- ① A person who wishes to use the equipment of UMCL must make a reservation and use the equipment after completing the training of the equipment manager, assessment test, and acquiring self-user qualification. (Analysis or process request is irrelevant to equipment training and qualification evaluation.)
- ② A user who completes the regular or occasional training (including practice) by the equipment manager can receive practical training from the senior student of his or her laboratory to improve proficiency before the assessment test. The qualification of the senior must be at least 1 year of experience (more than 5 times in the previous 6 months) in using the equipment. The laboratory is responsible for all safety and property issues arising from the practical training conducted by the senior student.

- ③ If there is no record of equipment used in the last 90 days, the qualification for self-use ends. A person who wants to reacquire the self-user qualification must receive equipment training and pass the assessment test conducted by the equipment manager. The upgrading for self-user can be made on the website of UCRF. (http://ucrf.unist.ac.kr)
- 4 Equipment reservations or requests can be made on the UNIST Portal System and the website of UCRF, and the reservation time should not be unnecessarily occupied for a long time so it does not affect the opportunity for others.
- ⑤ A user should be familiar with the safety rules for each equipment before using, and use the equipment after wearing appropriate safety gear.
- 6 Bringing chemicals and other items for personal use should be consulted with the equipment manager.
- 7 A user must check that there is no problem before using equipment, chemicals, and etc. If there is a problem before or after use, a user should promptly report to the equipment manager.
- ® A user must thoroughly fill out the "Performance Records" after using the equipment.
- (9) A user must take safety measures by posting the contents of the experiment to deliver accurate information to others if he inevitably leaves his seat during the experiment.
- ① The laboratory(in case of outsiders, affiliated institution) of self-user shall be obligated to compensate for all safety and property damage such as accidents (equipment damage, breakdowns, losses, etc.) caused by the negligence of the self-user.

#### Article 4. Cancellation after equipment reservation

- ① A self-user can cancel equipment reservation by himself up to 2 hours before equipment reservation time. However, TEM (HR-TEM, FE-TEM, Normal TEM, Bio-TEM) can be canceled up to 4 hours before. (※ Cancellation is not possible after the cancellation deadline has passed.)
- ② If a user has reserved an analysis request but wants to cancel it, he must notify the equipment manager at least 24 hours in advance. (However, in the case of NMR, notification would be allowed up to 1 hour left.) A user who does not appear at the reservation time without prior notice will be charged a usage fee for the reservation time.

### Article 5. Laboratory safety and user management

- ① A person who harms the safety of the laboratory or violates the rules of using the UMCL and damages the equipment use of another person, can be subject to penalties according to [Attached Table 1] and be taken appropriate action.
- ② If the violation of the rules is deliberately determined, the sanctions may be strengthened. If a user voluntarily declares after violating the rules, the sanctions may be eased.
- ③ If it is judged that the sanctions are difficult to be properly implemented due to the status of the violator (graduation or resignation), the user may be blocked from accessing UMCL.
- ④ A person who damages the property and facilities of UMCL by violating the rules shall be held liable to compensate for the damage.



⑤ If a violator does not follow the sanctions, the advisor of the violator will be held jointly responsible. (In the case of an outsider, the supervisor in charge of the affiliated institution)

# **Self-user Penalty**

#### 1. Criteria for penalty points

① A user shall be fined the penalty points in the event that any inappropriate behavior falls under the following. Each penalty item may be counted multiple times. (The expiration of penalty points is 1 year from the date of imposition.)

No.	Case description	Penalty points
1	Equipment is used by an unpermitted user who does not have a qualification of self-user.	5
2	Equipment is used without reservation (Including excessive use of equipment without additional reservation	3
3	A user operates an unpermitted function of the equipment	
4	An abnormality or malfunction discovered before or after using the equipment did not immediately reported to the manager	3
5	Damage, malfunction, and loss of equipment due to user negligence (* The user is responsible for all costs incurred due to the negligence. *)	5
6	A user does not provide the accurate information of the sample to the equipment manager, which is essential for protecting the safety, equipment or facilities	3
7	A person causes the leakage of a harmful substance, gas, or any risk of fire	5
8	A person uses or occupies the public items and other person's items without prior consent	1
9	A person leaves the laboratory without switching off the lights, locking the doors, tidying up the area, etc. after using equipment	1
10	A person does not follow the common lab safety rules(including clothing, prohibition of eating, etc.)	1



# **Self-user Penalty**

#### 2. Actions taken after subjecting penalty points

- ① If the cumulative penalty points exceed a certain criterion, the action corresponding with the table below will be taken.
- ② When a user violates the rule, an official letter from UCRF is sent to the department or institution(in case of the user outside) of the violator.
- ③ Even if the following actions have been taken due to the sum of the penalty points, the penalty points within the validity period(1 year) are effective.

Туре	Penalty points	Action
Total penalty points	5 points or more	<ul> <li>The user is prohibited from using the equipment for 1 month.</li> <li>When the prohibition period is finished, the user must complete the training and assessment again.</li> </ul>
awarded to 1 user	8 points or more	<ul> <li>The user is prohibited from using the equipment for 3 months.</li> <li>When the prohibition period is finished, the user must complete the training and assessment again.</li> </ul>
Total penalty points awarded to 1 laboratory	12 points or more	- Notify the user and the advisor(supervisor) by e-mail that "If the penalty score is more than 15 points, the members of your laboratory are prohibited from using the equipment for 1 month."
for 1 equipment	15 points or more	<ul> <li>The members of the laboratory are prohibited from using the equipment for 1 month</li> <li>Send an official letter of action to the affiliated department(institution)</li> </ul>





# THANK YOU